

Sample Name : DYKDDDDK Peptide  
 Cat. No. : RP10586  
 Lot. No. : PE8921603

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

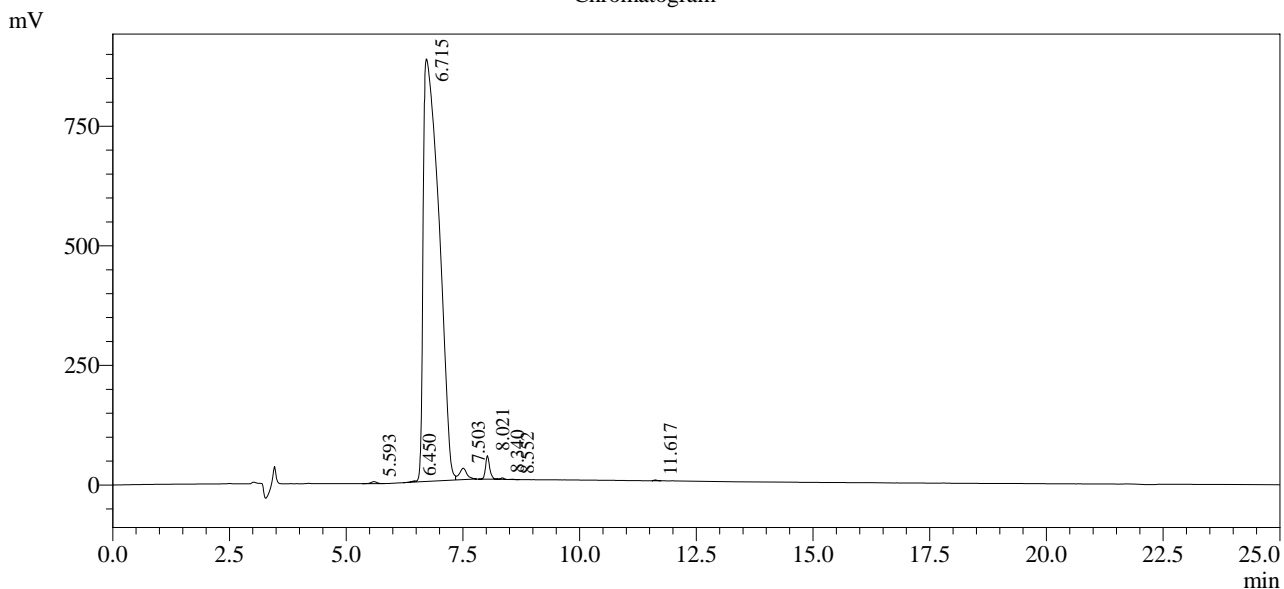

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.593	35181	4108	0.165
2	6.450	11544	2288	0.054
3	6.715	20667224	883467	96.965
4	7.503	271349	23999	1.273
5	8.021	300783	49082	1.411
6	8.340	15733	3073	0.074
7	8.552	3815	810	0.018
8	11.617	8490	1672	0.040
Total		21314120	968499	100.000