

Sample Name : Hexa-His
 Cat. No. : RP11737
 Lot. No. : PE9451604

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

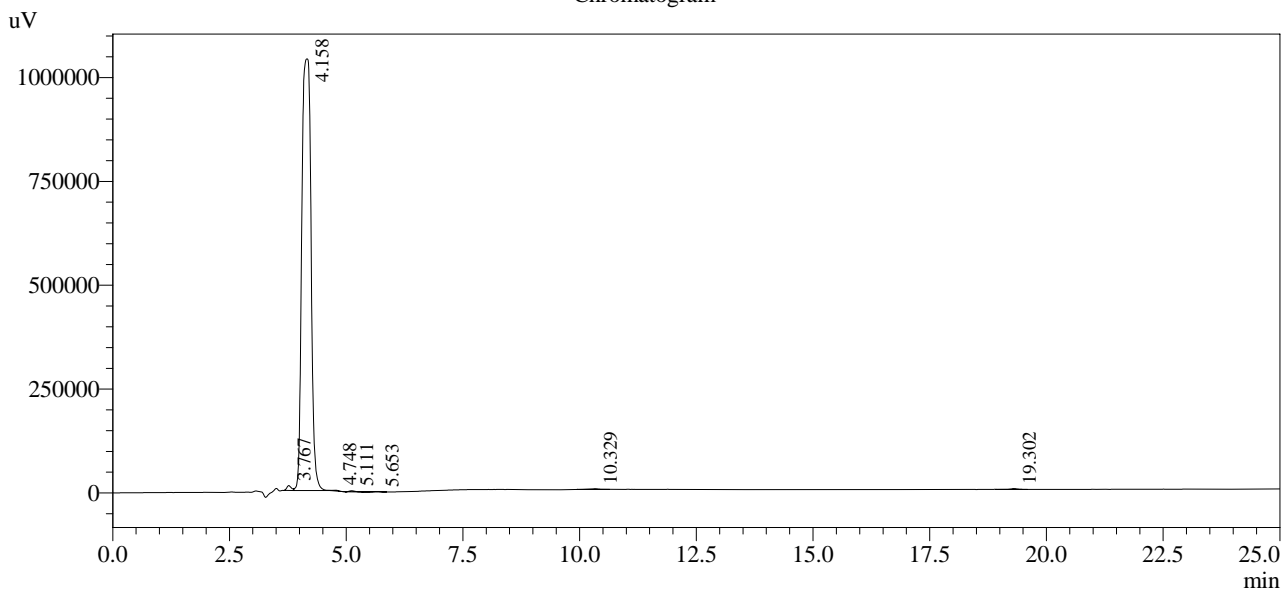

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	3.767	78926	11869	0.548
2	4.158	14236806	1039197	98.865
3	4.748	16488	2112	0.114
4	5.111	23116	2579	0.161
5	5.653	14023	1413	0.097
6	10.329	15754	1353	0.109
7	19.302	15140	1786	0.105
Total		14400253	1060309	100.000