

Sample Name : OVA Peptide (257-264)
 Sample ID : C3601BG280-1

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

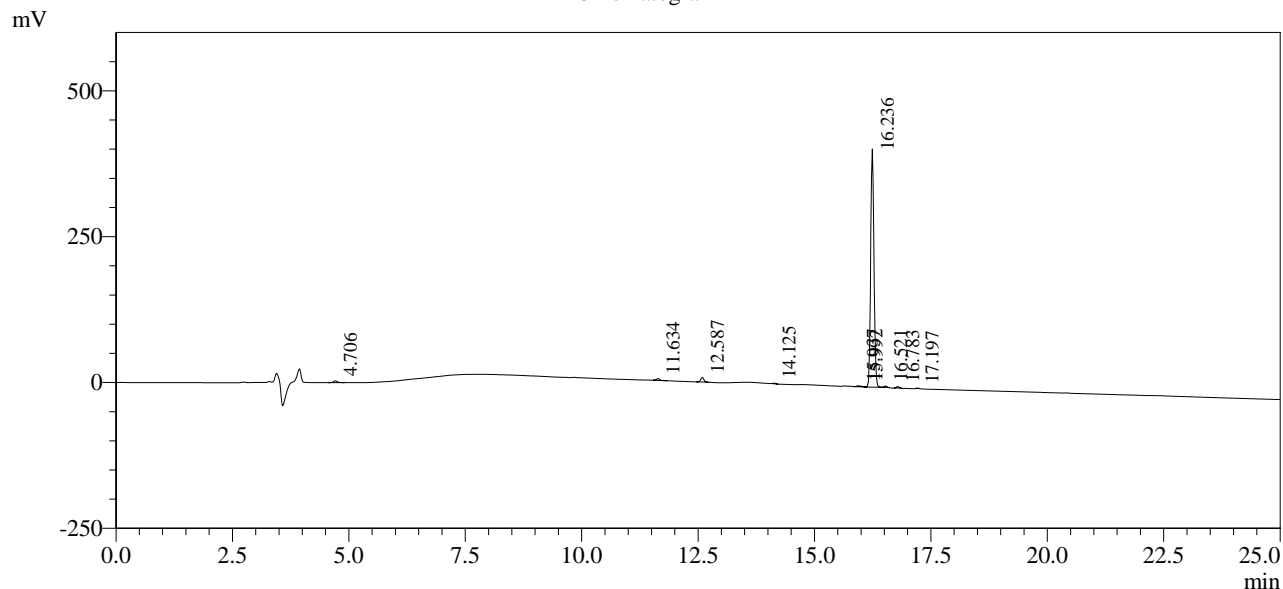

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	4.706	18286	3103	0.869
2	11.634	15186	3116	0.722
3	12.587	36898	7964	1.754
4	14.125	2979	851	0.142
5	15.937	7770	1569	0.369
6	15.992	4336	1234	0.206
7	16.236	1999355	408462	95.020
8	16.521	7560	2037	0.359
9	16.783	10216	2473	0.486
10	17.197	1547	561	0.074
Total		2104133	431370	100.000