


Mass Spectrum

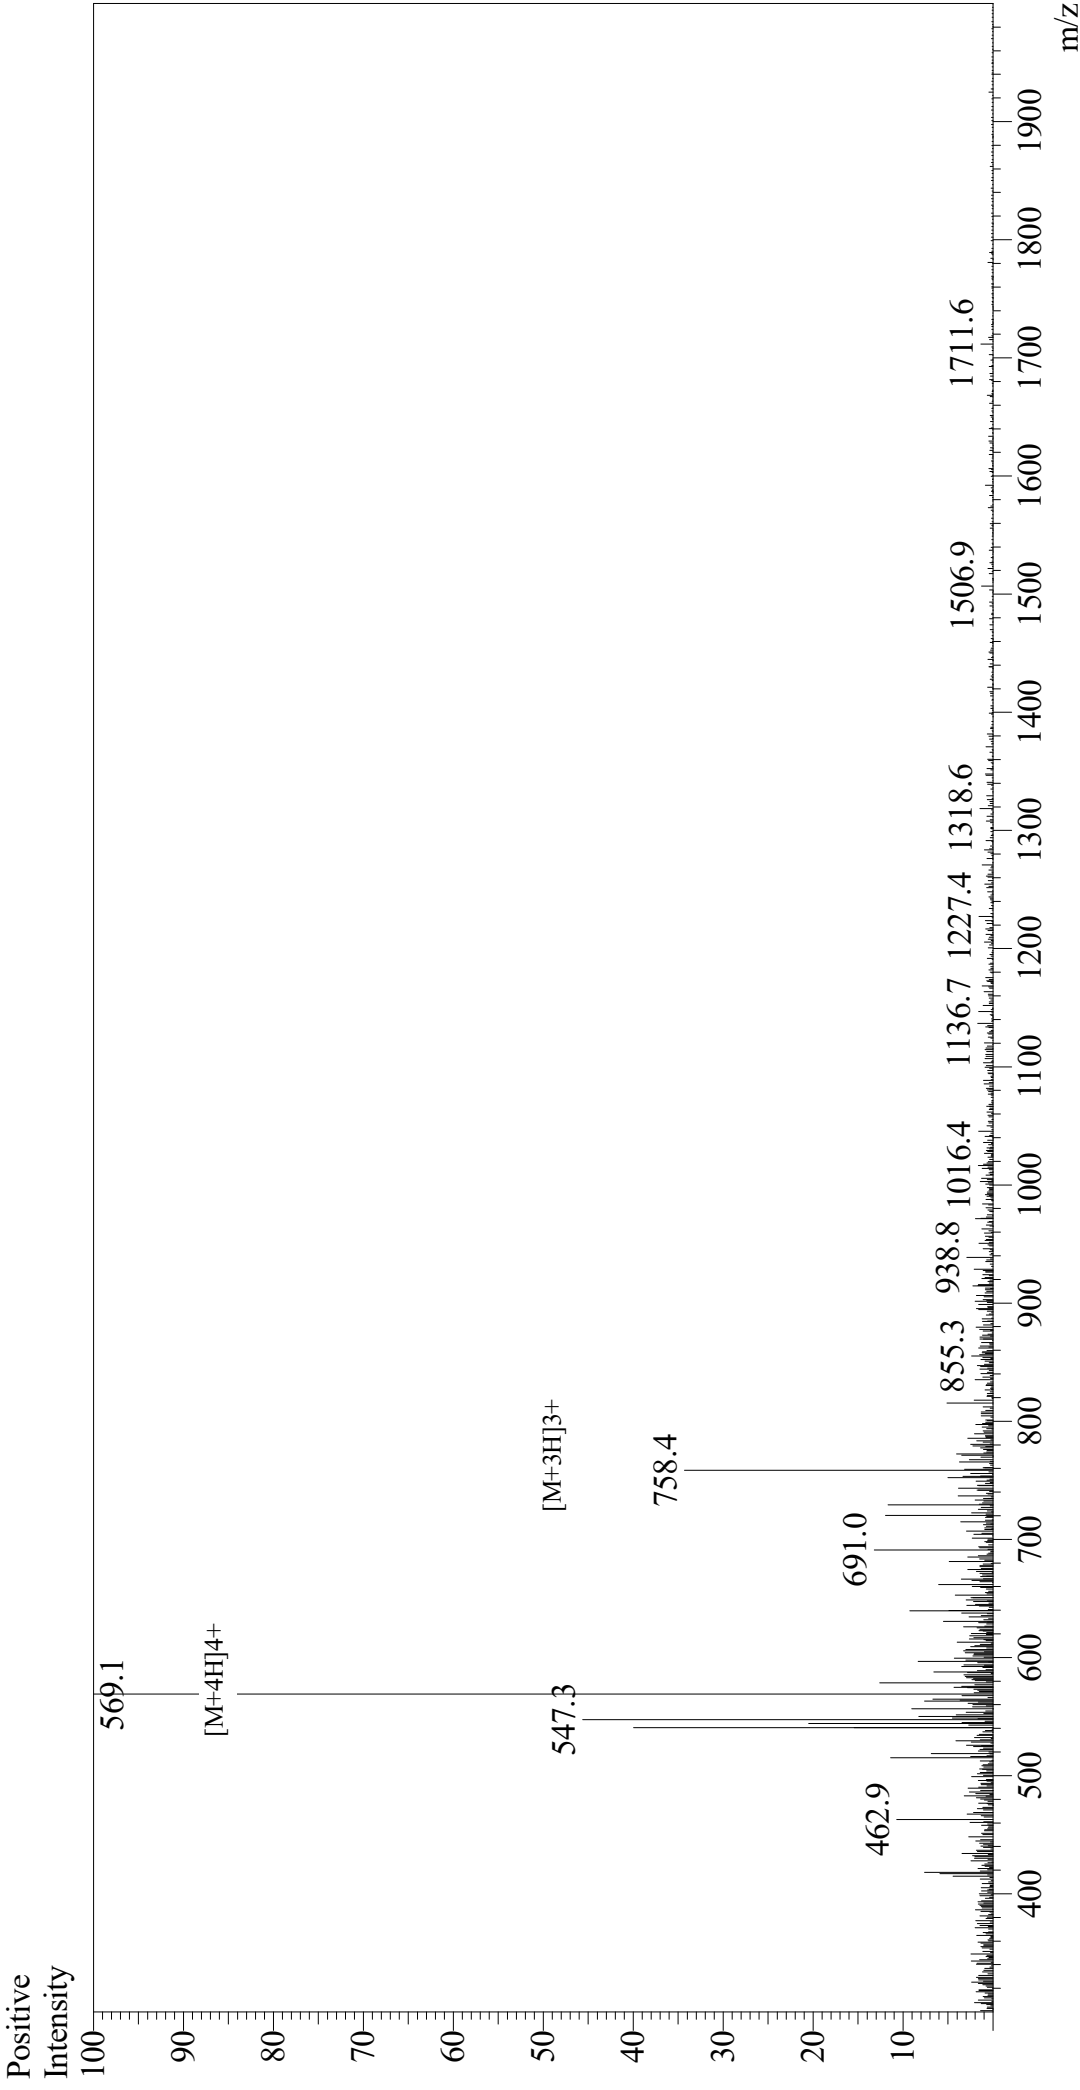

Sample Information

Acquired by : Gary
 Month-Day Processed : 12/26/19
 Time Processed : 09:33:42 AM
 Injection Volume : 0.3
 Sample Name : Flagelin22
 Cat. No. : RP19986
 Lot. No. : E1827319L
 Theoretical MW : 2272.50
 Observed MW : 2272.4

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : GK11010007
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H_2O /50% MeOH