

Sample Name :Hexa-His  
 Cat. No. :RP11737  
 Lot. No. :PE9861607

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

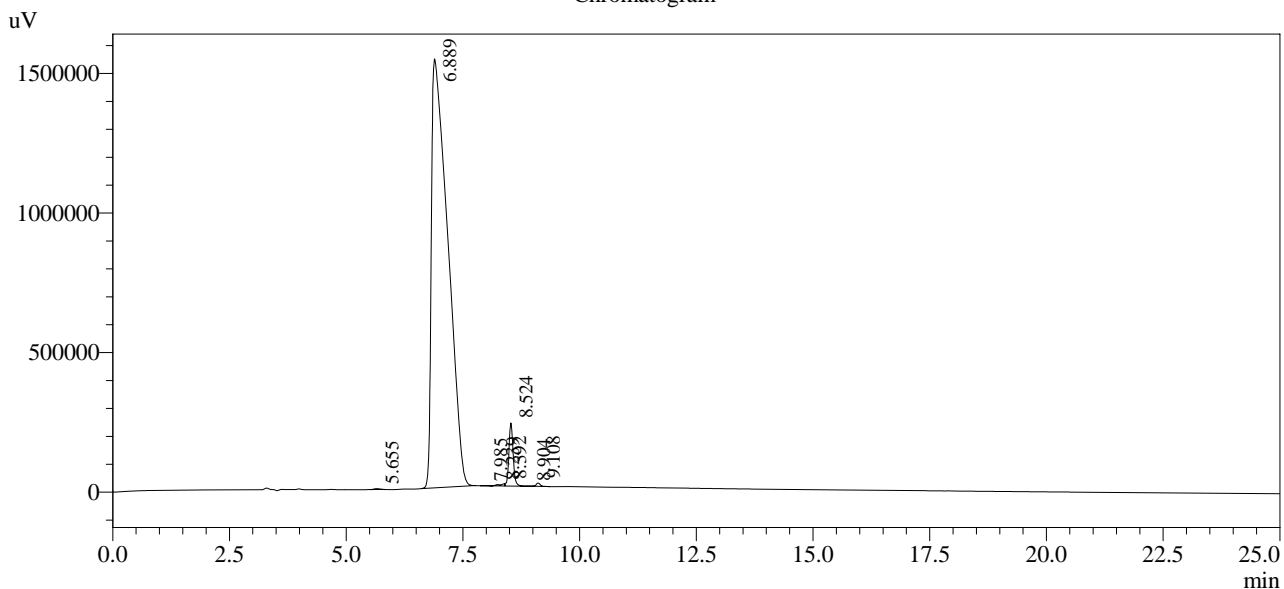

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.655	28424	3113	0.073
2	6.889	37531153	1537000	95.934
3	7.985	2528	357	0.006
4	8.239	31360	4643	0.080
5	8.392	36539	8274	0.093
6	8.524	1418790	226042	3.627
7	8.904	1482	357	0.004
8	9.108	71634	12102	0.183
Total		39121911	1791889	100.000