

Sample Name : LAH4  
 Cat. No. : RP20026  
 Lot. No. : PE5621607


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

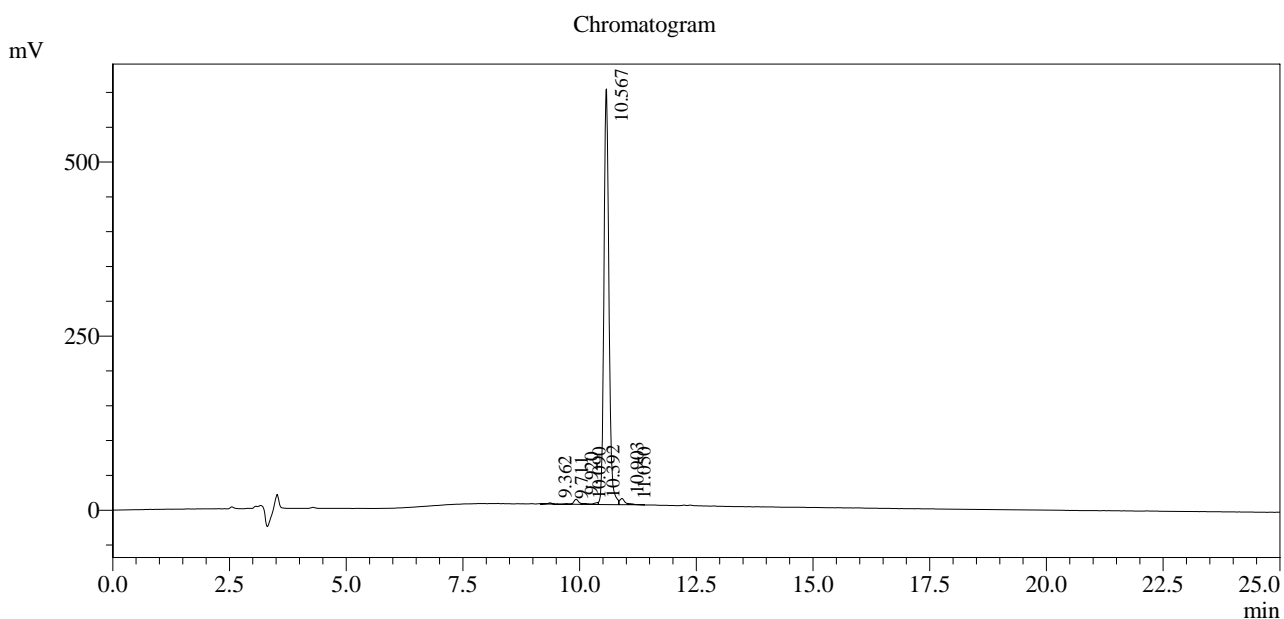

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.362	8945	1596	0.195
2	9.711	2773	478	0.060
3	9.920	50724	7229	1.104
4	10.090	9822	1272	0.214
5	10.392	17499	2852	0.381
6	10.567	4428056	597116	96.381
7	10.903	64145	8930	1.396
8	11.050	12376	1652	0.269
Total		4594340	621125	100.000