

Sample Name :RGD
 Cat No. :RP20297
 Lot No. :E2123819L
 Time Processed :16:58:20
 Month-Day-Year Processed :12/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

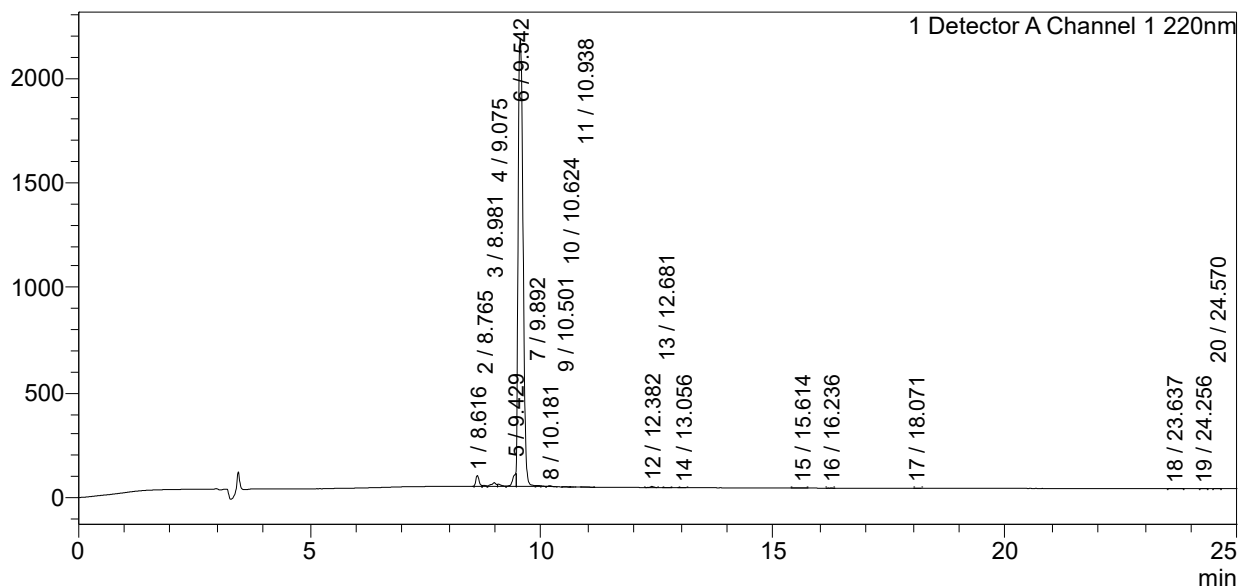

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.616	250804	52279	1.521
2	8.765	21216	4218	0.129
3	8.981	121021	17438	0.734
4	9.075	60330	10289	0.366
5	9.429	238309	55081	1.445
6	9.542	15718541	2136696	95.325
7	9.892	1253	365	0.008
8	10.181	22016	4608	0.134
9	10.501	7261	1418	0.044
10	10.624	3386	770	0.021
11	10.938	5039	638	0.031
12	12.382	25346	5022	0.154
13	12.681	2056	406	0.012
14	13.056	1176	198	0.007
15	15.614	2759	311	0.017

Peak#	Ret. Time	Area	Height	Area%
16	16.236	1983	312	0.012
17	18.071	1370	263	0.008
18	23.637	2692	225	0.016
19	24.256	1820	270	0.011
20	24.570	1086	276	0.007
Total		16489465	2291082	100.000