

Sample Name : β -Amyloid (1-40)
 Cat. No. : RP10004
 Lot. No. : PE2001609

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

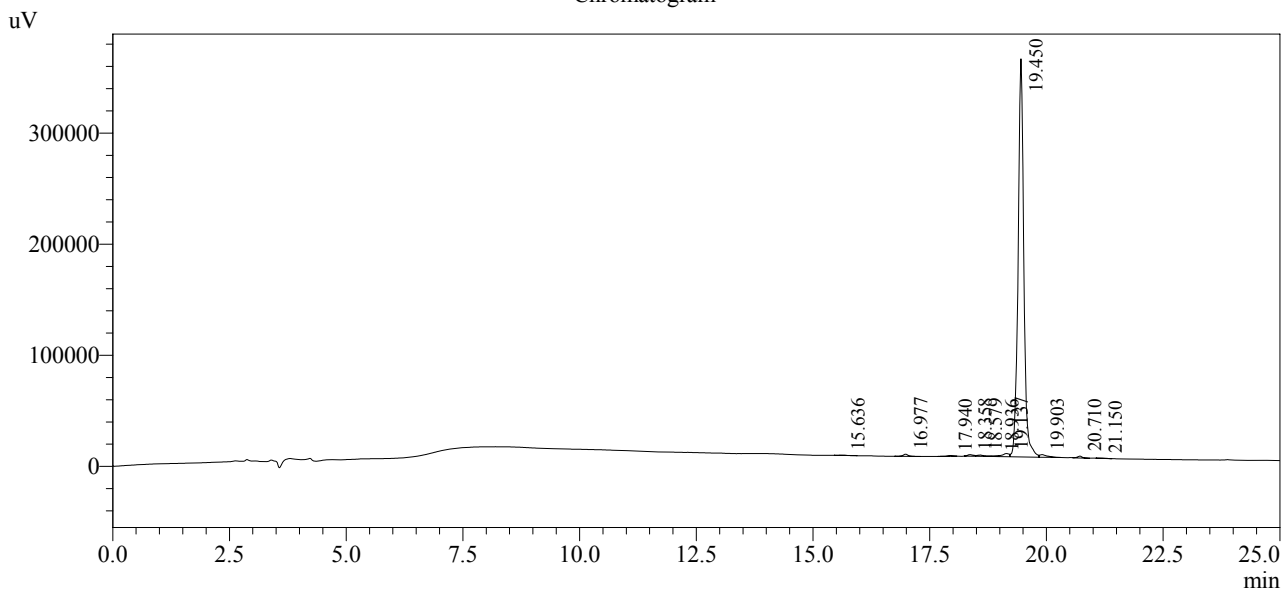

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.636	4301	375	0.135
2	16.977	15740	1982	0.493
3	17.940	5274	525	0.165
4	18.358	12349	1390	0.387
5	18.579	13670	1126	0.428
6	18.936	6762	875	0.212
7	19.137	28409	2831	0.890
8	19.450	3064933	358214	96.016
9	19.903	25985	2285	0.814
10	20.710	11731	1661	0.367
11	21.150	2948	291	0.092
Total		3192101	371553	100.000