


Mass Spectrum

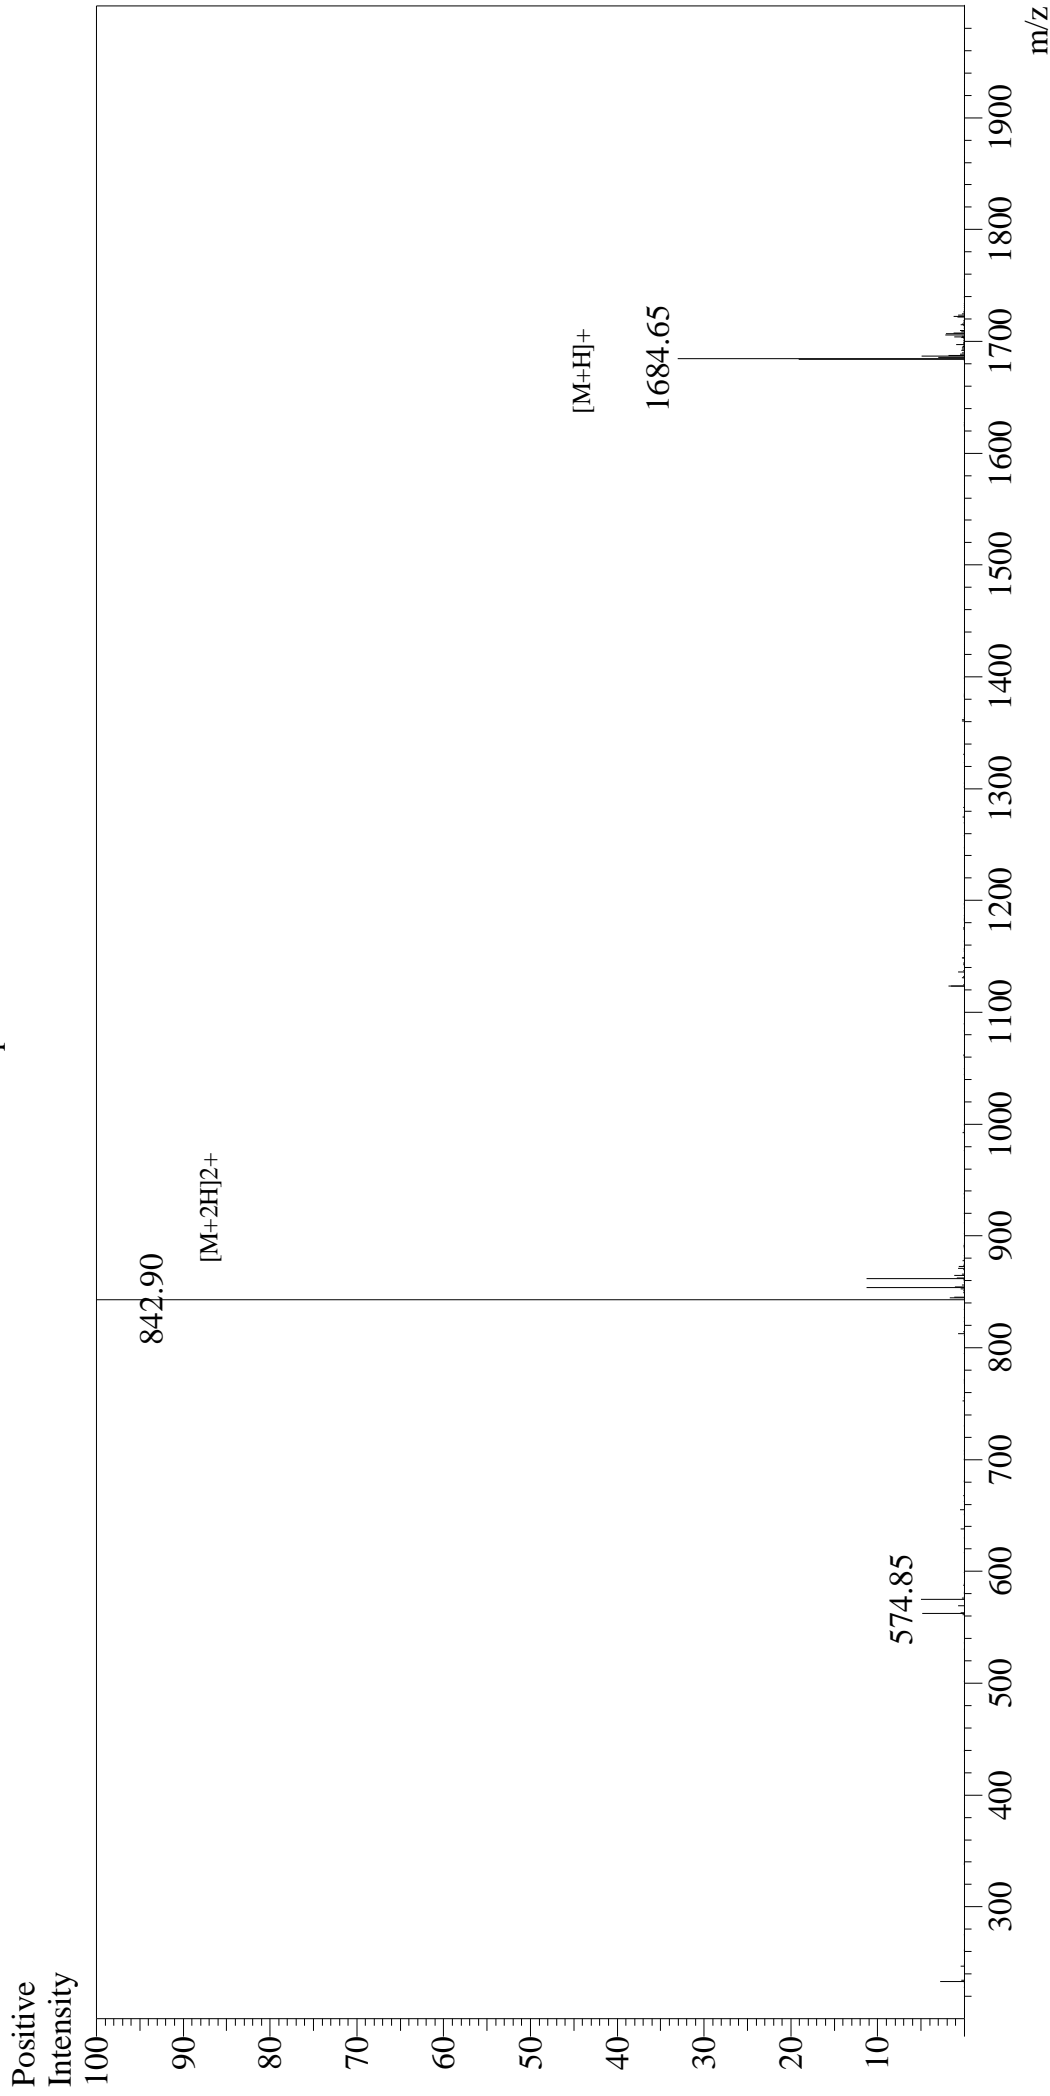

Sample Information

User : Gary
Month-Day Processed : 07/22/16
Time Processed : 13:56:56
Injection Volume : 0.2
Sample Name : α -factor pheromone for yeast
Cat No. : RP01002
Lot No. : PE6721607
Theoretical MW : 1683.98
Observed MW : 1683.80

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH