

Sample Name :  $\beta$ -Amyloid (1-42), human  
 Cat. No. : RP10017  
 Lot. No. : PE1061601


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	10	
25.00	Pumps	Pump B Conc.	100	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	10	
40.00	Pumps	Pump B Conc.	10	
41.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima<sup>TM</sup> C18 4.6 x 250 mm

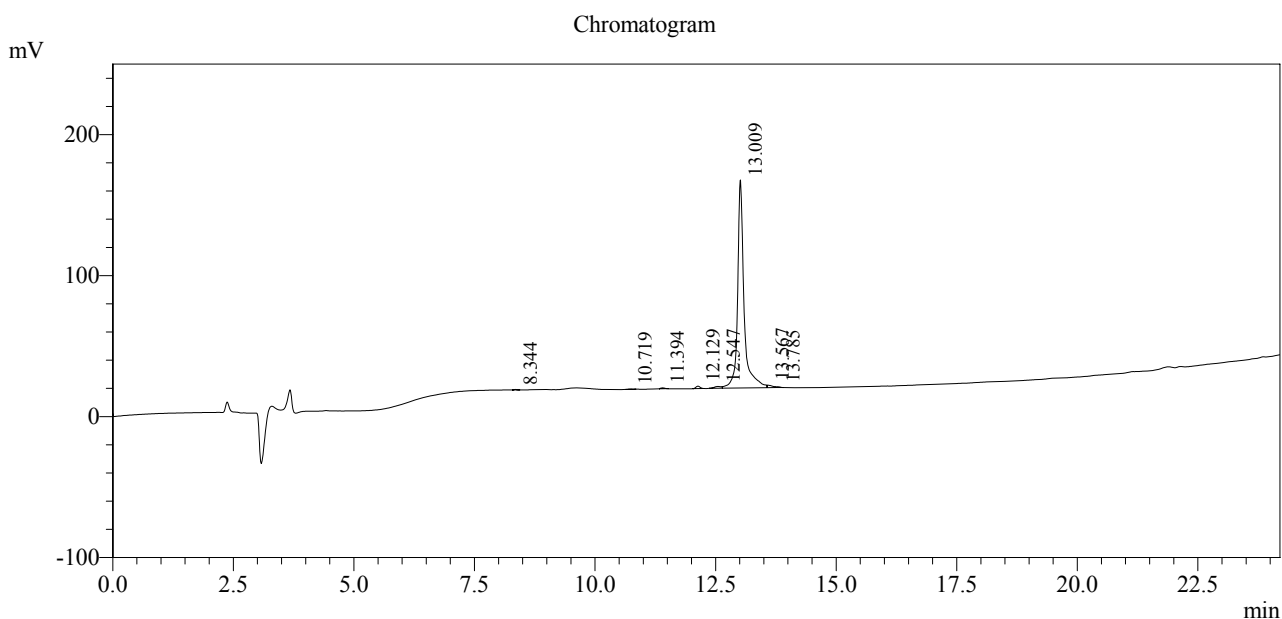

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.344	1119	375	0.079
2	10.719	1030	211	0.073
3	11.394	3423	579	0.242
4	12.129	10466	1754	0.741
5	12.547	13103	1294	0.928
6	13.009	1367284	147596	96.802
7	13.567	13086	1829	0.926
8	13.785	2937	551	0.208
Total		1412447	154189	100.000