

Sample Name :C-Peptide (3-33), human
Cat. No. :RP11116
Lot. No. : PE7711607

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
10.00	Pumps	Pump B Conc.	35	
35.00	Pumps	Pump B Conc.	95	
41.00	Pumps	Pump B Conc.	95	
41.01	Pumps	Pump B Conc.	5	
50.00	Pumps	Pump B Conc.	5	
50.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

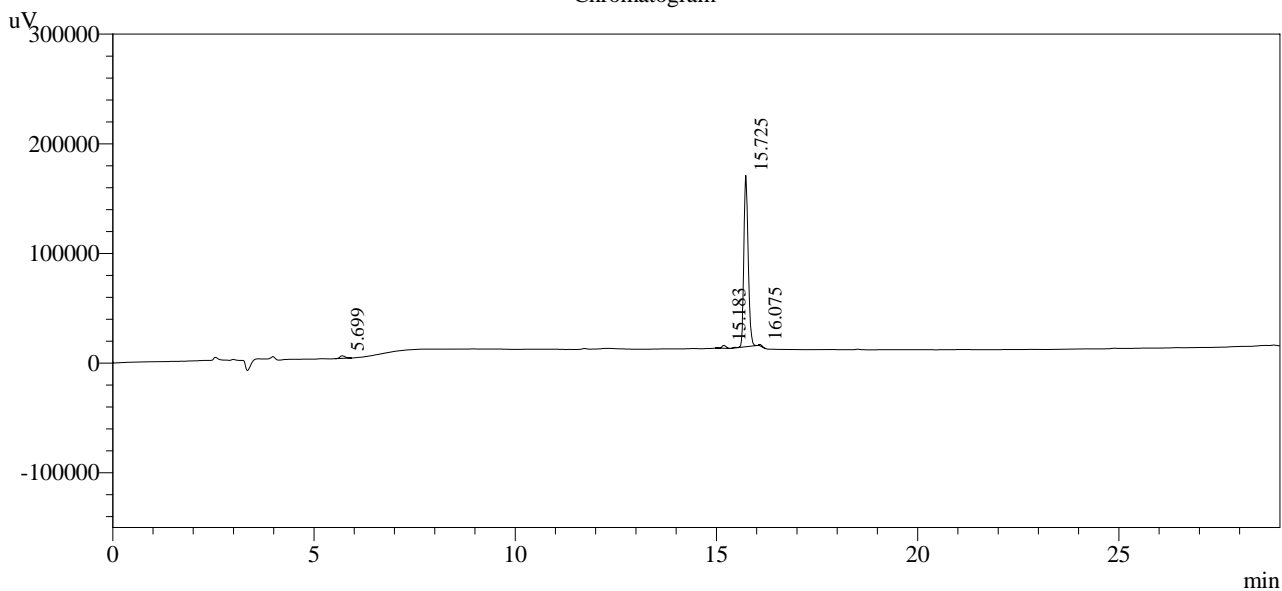

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.699	20895	2310	1.703
2	15.183	19060	2617	1.554
3	15.725	1180504	156398	96.239
4	16.075	6179	1184	0.504
Total		1226637	162509	100.000