

Sample Name : Hexa-His
 Cat. No. : RP11737
 Lot. No. : PE5391607

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

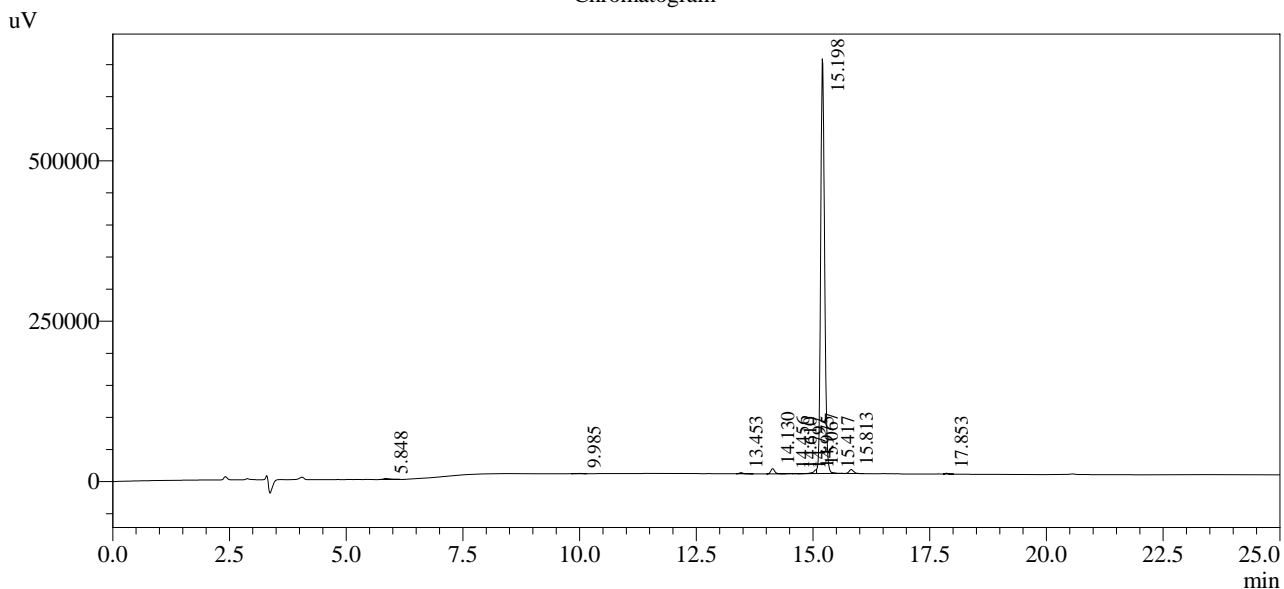

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.848	10622	1532	0.270
2	9.985	5459	833	0.139
3	13.453	10093	1783	0.256
4	14.130	48166	8177	1.223
5	14.456	2845	562	0.072
6	14.610	574	137	0.015
7	14.797	1136	203	0.029
8	14.975	6623	1308	0.168
9	15.067	23586	6159	0.599
10	15.198	3778460	646387	95.911
11	15.417	5075	1231	0.129
12	15.813	41670	6279	1.058
13	17.853	5237	1153	0.133
Total		3939546	675743	100.000