

Sample Name : GRGDSPC  
 Cat. No. : RP20283  
 Lot. No. : PE9911707

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

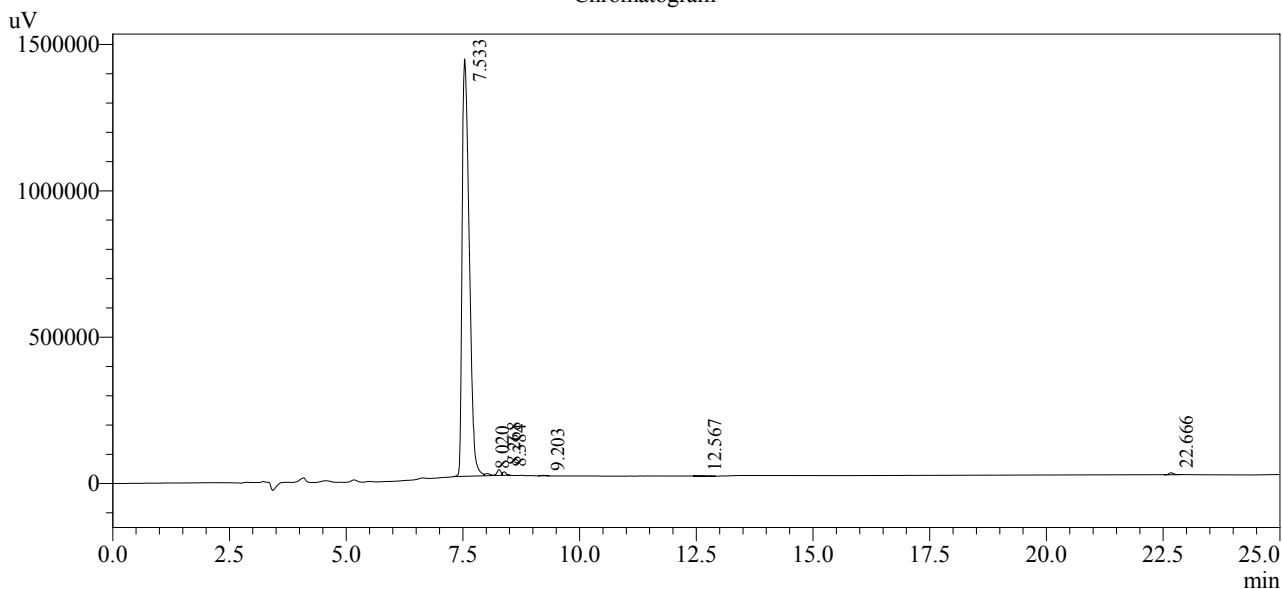

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.533	15152288	1426444	98.100
2	8.020	57934	7487	0.375
3	8.268	117100	19680	0.758
4	8.384	56283	11671	0.364
5	9.203	10309	1491	0.067
6	12.567	7396	942	0.048
7	22.666	44524	6404	0.288
Total		15445834	1474120	100.000