

Sample Name : $\beta$ -Amyloid (1-42), human  
 Cat No. :RP10017  
 Lot No. :PE4341905  
 Time Processed :10:54:38  
 Month-Day-Year Processed :05/31/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010141

### <Chromatogram>

mV

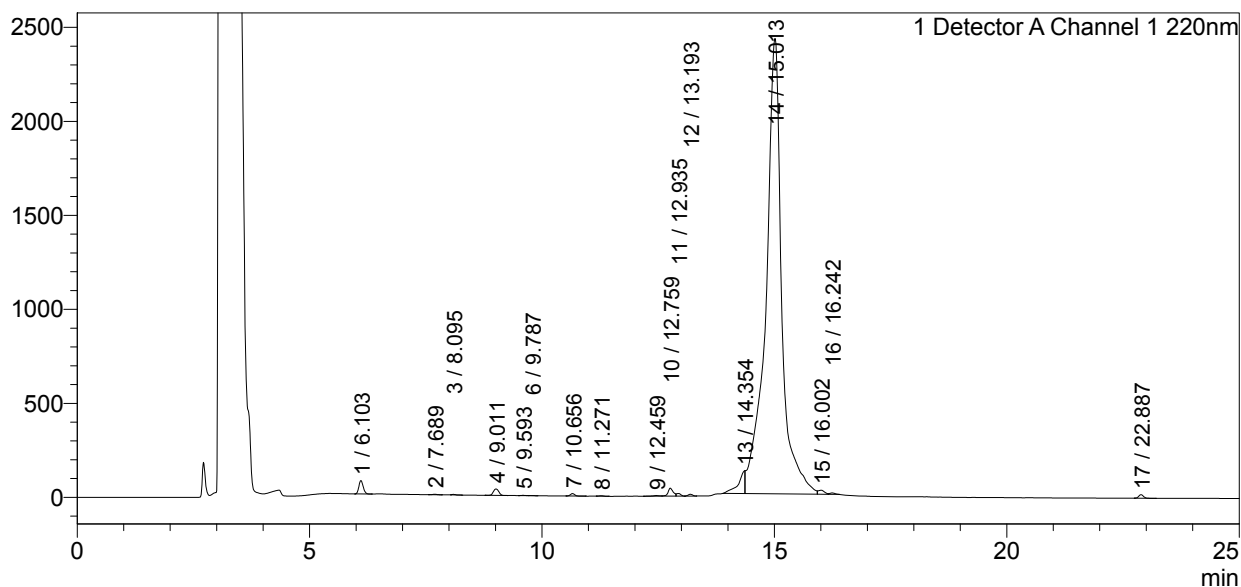

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.103	464013	71236	0.769
2	7.689	16292	2766	0.027
3	8.095	11834	2696	0.020
4	9.011	281323	34244	0.466
5	9.593	9365	1618	0.016
6	9.787	5152	1034	0.009
7	10.656	81150	12740	0.134
8	11.271	14759	2379	0.024
9	12.459	34927	3470	0.058
10	12.759	323981	42590	0.537
11	12.935	86321	14124	0.143
12	13.193	64720	9644	0.107
13	14.354	1211355	120004	2.008
14	15.013	57354529	2421676	95.055
15	16.002	196753	21139	0.326

Peak#	Ret. Time	Area	Height	Area%
16	16.242	53810	7138	0.089
17	22.887	127865	18717	0.212
Total		60338147	2787214	100.000