

Sample Name : Cortistatin 14, human, rat  
 Cat. No. : RP10972  
 Lot. No. : E9486120B  
 Time Processed : 9:50:44  
 Month-Day-Year Processed : 02/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

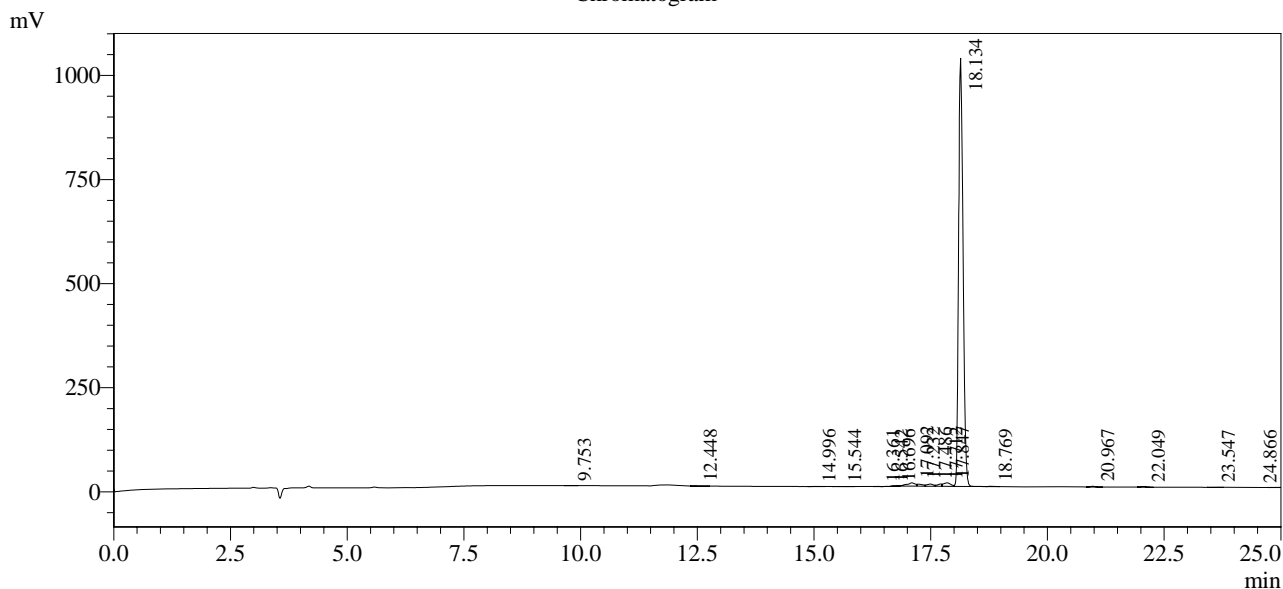

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.753	2008	153	0.028
2	12.448	1430	117	0.020
3	14.996	1066	78	0.015
4	15.544	2460	227	0.034
5	16.361	1996	347	0.027
6	16.542	378	50	0.005
7	16.696	5770	1186	0.079
8	17.092	98404	7881	1.354
9	17.232	42357	4665	0.583
10	17.486	50804	5270	0.699
11	17.712	36967	5533	0.508
12	17.847	88590	8268	1.219
13	18.134	6909401	1028270	95.040
14	18.769	4466	774	0.061
15	20.967	11350	1774	0.156
16	22.049	9285	1289	0.128
17	23.547	1247	99	0.017
18	24.866	2024	272	0.028
Total		7270006	1066254	100.000