

Sample Name : Ghrelin, rat
 Cat. No. : RP10781
 Lot. No. : E6464620A
 Time Processed : 8:48:46
 Month-Day-Year Processed : 02/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

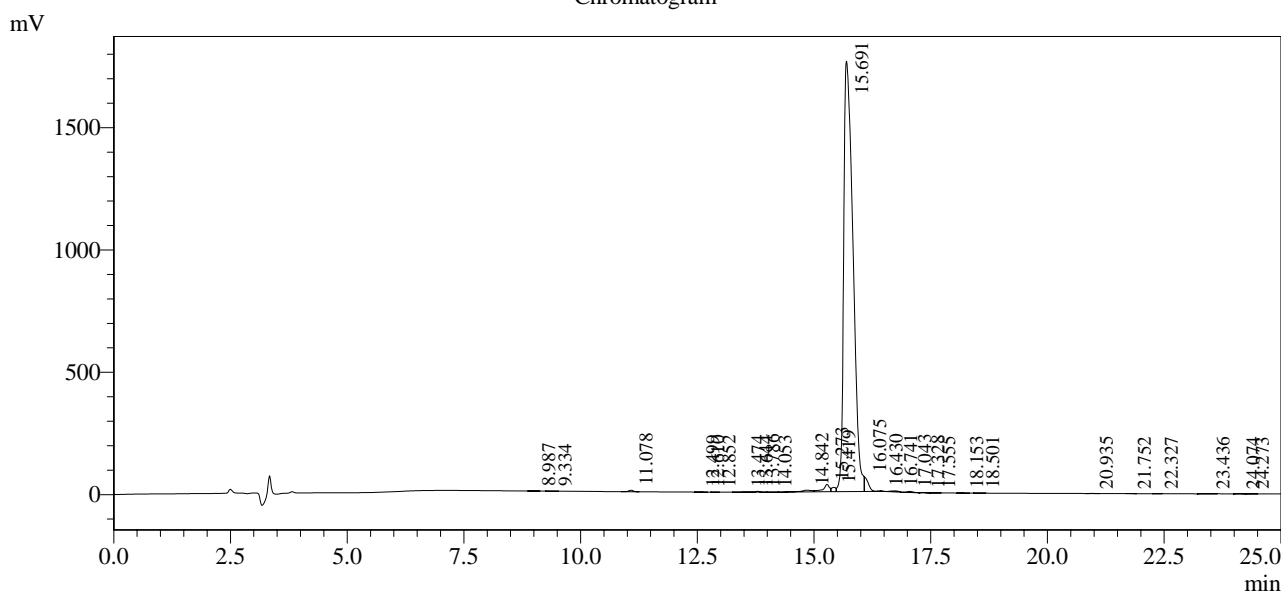

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.987	4167	591	0.016
2	9.334	1702	275	0.007
3	11.078	41761	6330	0.165
4	12.499	2066	325	0.008
5	12.610	1499	347	0.006
6	12.852	2370	412	0.009
7	13.474	7340	660	0.029
8	13.644	5145	668	0.020
9	13.786	23315	3634	0.092
10	14.053	2585	277	0.010
11	14.842	123594	7178	0.487
12	15.273	279476	29722	1.102
13	15.419	112725	17755	0.444
14	15.691	24294610	1759303	95.757
15	16.075	336886	61187	1.328
16	16.430	14590	2820	0.058
17	16.741	48490	4096	0.191
18	17.043	39584	4499	0.156
19	17.328	8046	1506	0.032
20	17.555	1346	182	0.005
21	18.153	3654	479	0.014
22	18.501	1919	267	0.008
23	20.935	2060	254	0.008
24	21.752	1096	135	0.004

Peak#	Ret. Time	Area	Height	Area %
25	22.327	1034	155	0.004
26	23.436	5007	326	0.020
27	24.074	3899	409	0.015
28	24.273	1243	136	0.005
Total		25371208	1903928	100.000