

Sample Name : β -Amyloid (1-42), human
 Cat No. : RP20527
 Lot No.: PE1031903
 Time Processed : 17:27:42
 Month-Day-Year Processed : 04/12/2019

Pump A : 0.5% Ammonia solution in 100% water (v/v)
 Pump B : 0.2% Ammonia solution in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
37.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : UniPS 10-300 4.6 x 250 mm

Equipment: GR09010180

Chromatogram

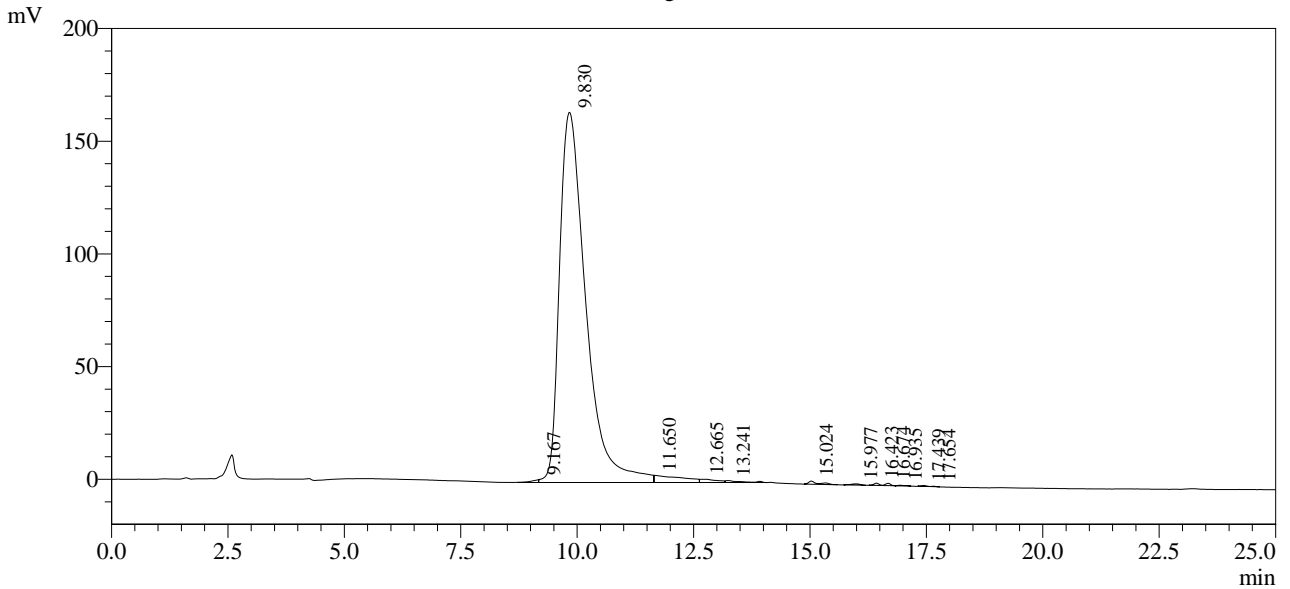

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.167	12964	1202	0.193
2	9.830	6453932	164266	96.227
3	11.650	132306	3232	1.973
4	12.665	37229	1473	0.555
5	13.241	21899	892	0.327
6	15.024	20360	1387	0.304
7	15.977	7317	537	0.109
8	16.423	7407	962	0.110
9	16.674	7587	1006	0.113
10	16.935	3306	295	0.049
11	17.439	1607	236	0.024
12	17.654	1096	178	0.016
Total		6707011	175666	100.000