

Sample Name :Substance P
 Cat No. :RP10178
 Lot No. :E1327121C
 Time Processed :11:17:58 AM
 Month-Day-Year Processed :03/24/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

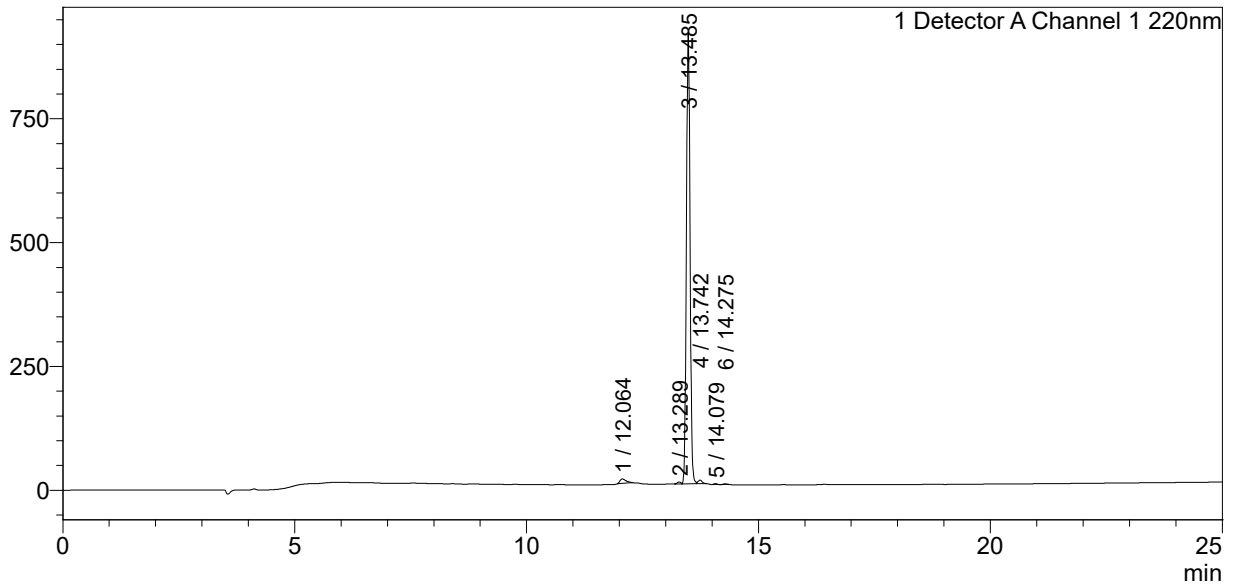

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.064	76301	8712	1.473
2	13.289	21666	3900	0.418
3	13.485	5023741	910032	97.014
4	13.742	42978	7202	0.830
5	14.079	6541	1550	0.126
6	14.275	7165	1451	0.138
Total		5178392	932847	100.000