

Sample Name : PAR-4 Agonist Peptide, amide  
 Cat.No : RP11529  
 Lot.No : E90285201  
 Time Processed: 7:03:51  
 Year-Month-Day: 2020/9/16

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min

<<Detector A>>  
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010015

<Chromatogram>

mV

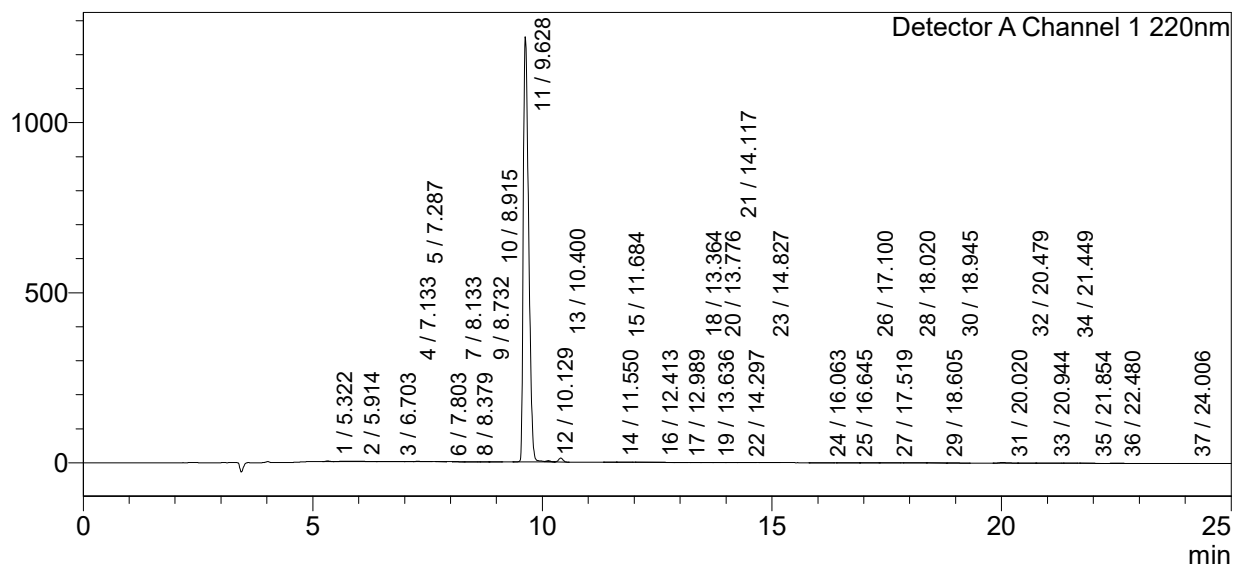

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.322	8253	1579	0.079
2	5.914	25831	815	0.246
3	6.703	7681	486	0.073
4	7.133	1118	143	0.011
5	7.287	8158	1194	0.078
6	7.803	1131	104	0.011
7	8.133	1261	151	0.012
8	8.379	1027	173	0.010
9	8.732	1138	180	0.011
10	8.915	2869	425	0.027
11	9.628	10206059	1250090	97.381
12	10.129	16173	2808	0.154
13	10.400	78339	12058	0.747
14	11.550	1860	179	0.018

Peak#	Ret. Time	Area	Height	Area%
15	11.684	3211	320	0.031
16	12.413	19450	721	0.186
17	12.989	2176	209	0.021
18	13.364	2644	311	0.025
19	13.636	4150	353	0.040
20	13.776	2976	403	0.028
21	14.117	2519	288	0.024
22	14.297	2282	190	0.022
23	14.827	1621	107	0.015
24	16.063	4038	205	0.039
25	16.645	7053	365	0.067
26	17.100	4539	318	0.043
27	17.519	3675	265	0.035
28	18.020	3528	228	0.034
29	18.605	3693	320	0.035
30	18.945	2507	176	0.024
31	20.020	25604	2146	0.244
32	20.479	5046	389	0.048
33	20.944	3152	201	0.030
34	21.449	1327	121	0.013
35	21.854	2499	241	0.024
36	22.480	9173	551	0.088
37	24.006	2772	382	0.026
Total		10480534	1279194	100.000