

Sample Name :Gastric Inhibitory Peptide (GIP), human
 Cat No. :RP10795
 Lot No. :E0845220H
 Time Processed :3:18:17
 Month-Day-Year Processed :08/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

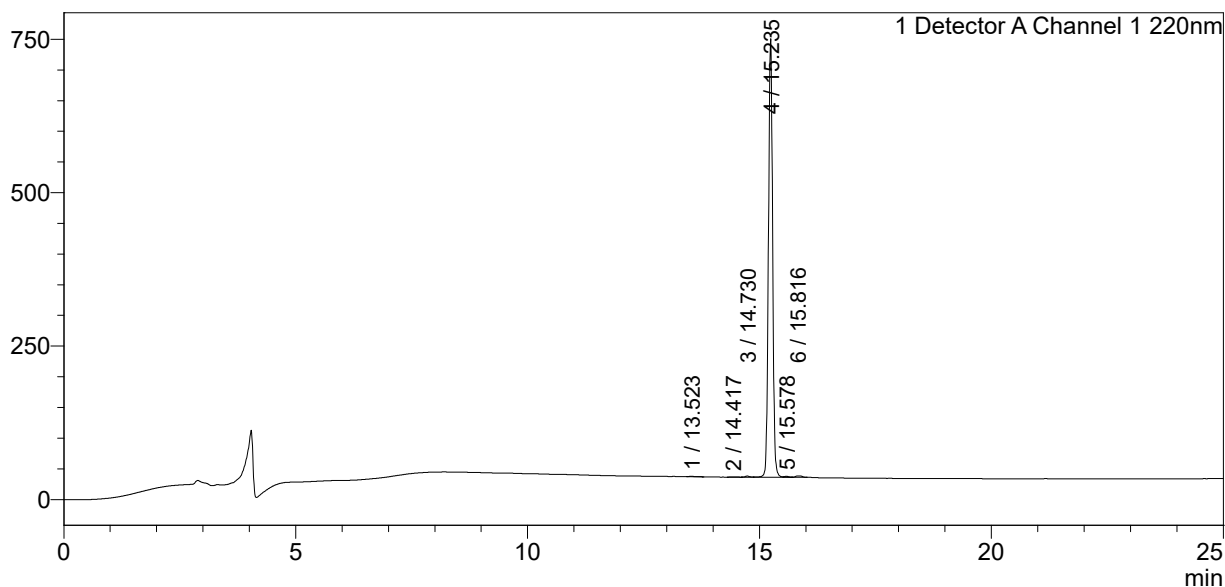

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.523	3948	478	0.088
2	14.417	3766	301	0.084
3	14.730	13181	1854	0.293
4	15.235	4453155	714832	98.953
5	15.578	5440	1124	0.121
6	15.816	20771	2091	0.462
Total		4500262	720680	100.000