


Mass Spectrum

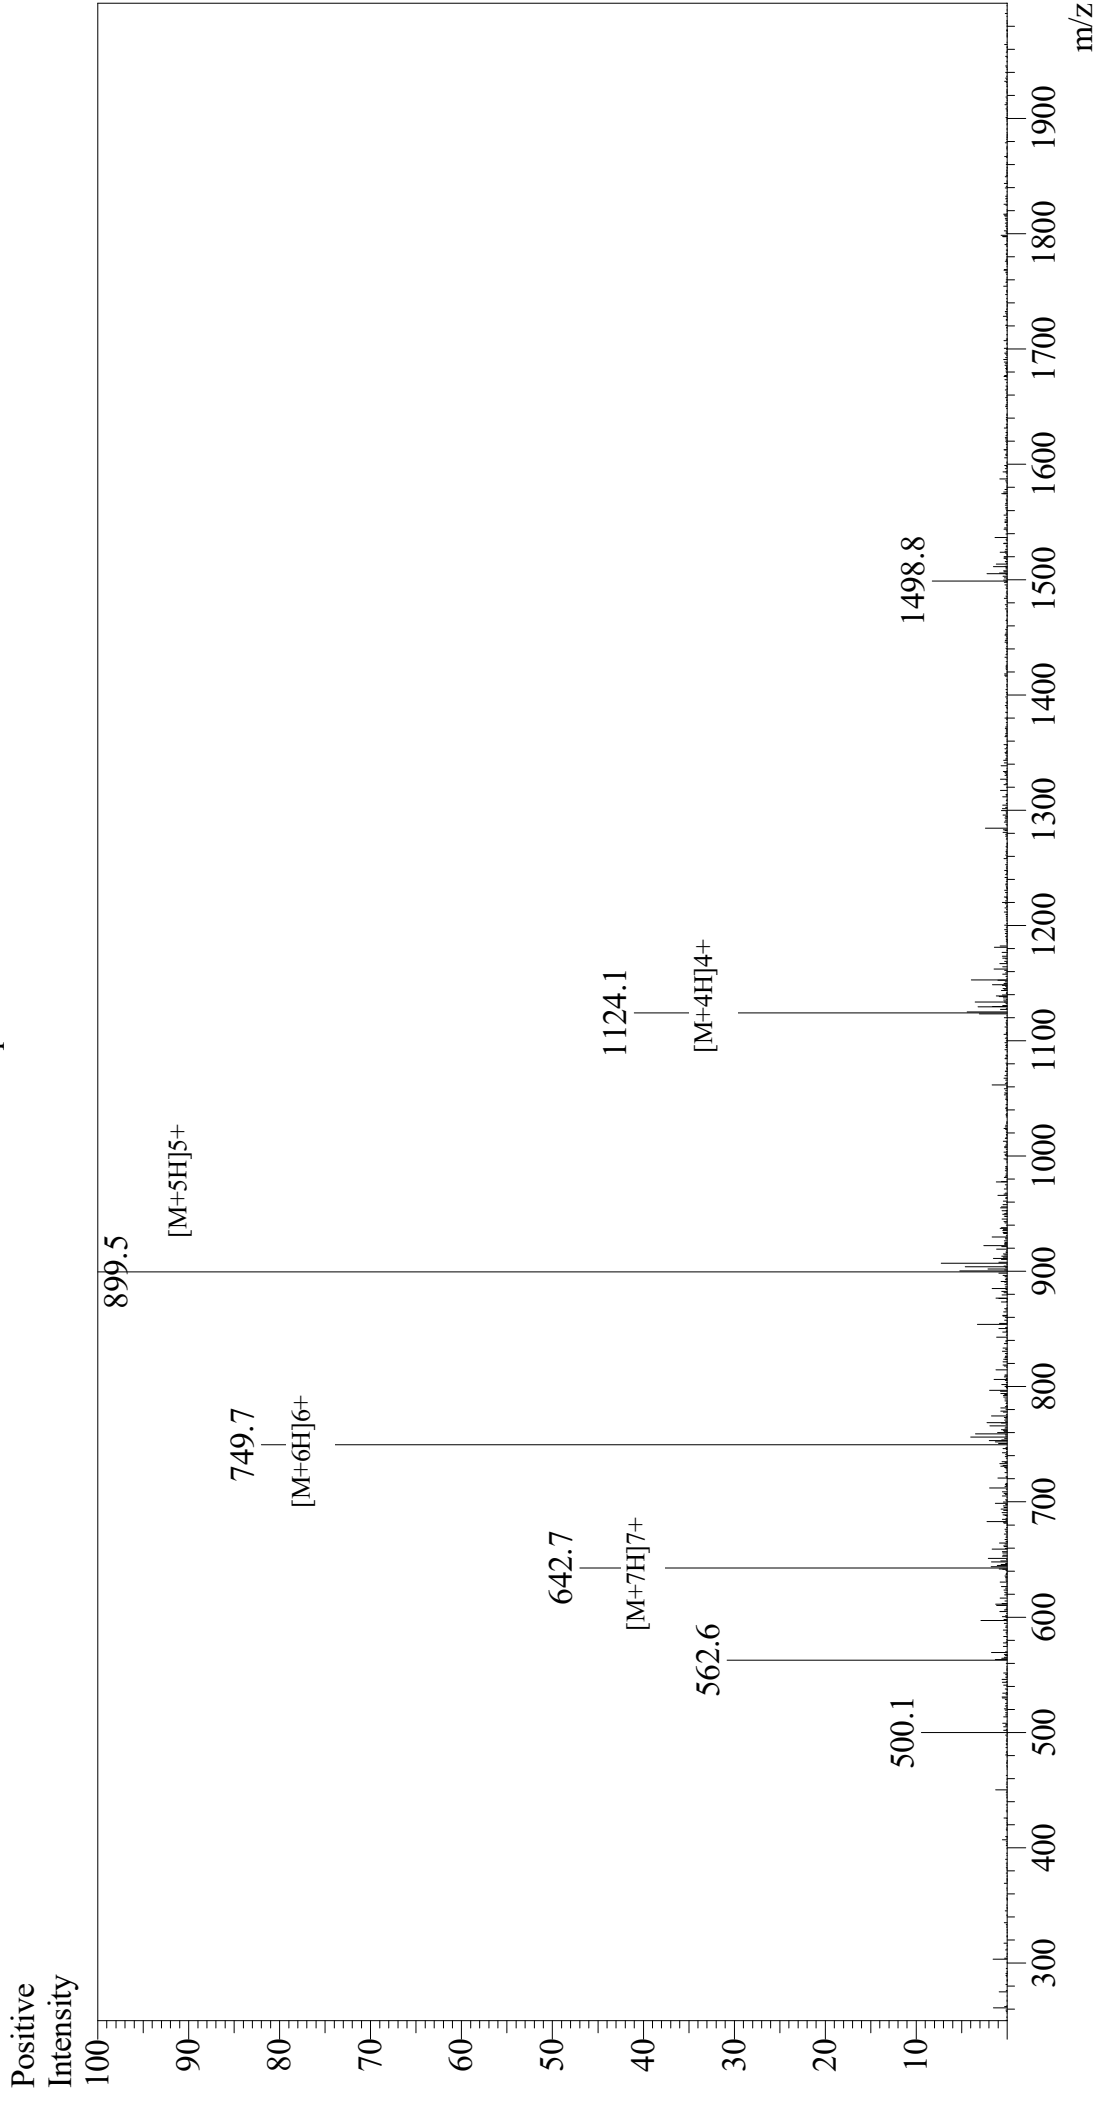

Sample Information
Month-Day Processed : 01/15/21
Time Processed : 8:27:04 AM
Injection Volume : 0.3
Sample Name : LL37 (Human)
Cat No. : RP13323
Lot No. : E7135021A
Theoretical MW : 4493.28
Observed MW : 4492.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeOH