

Sample Name :DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : E7833719J
 Time Processed :8:28:10
 Month-Day-Year Processed : 10/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

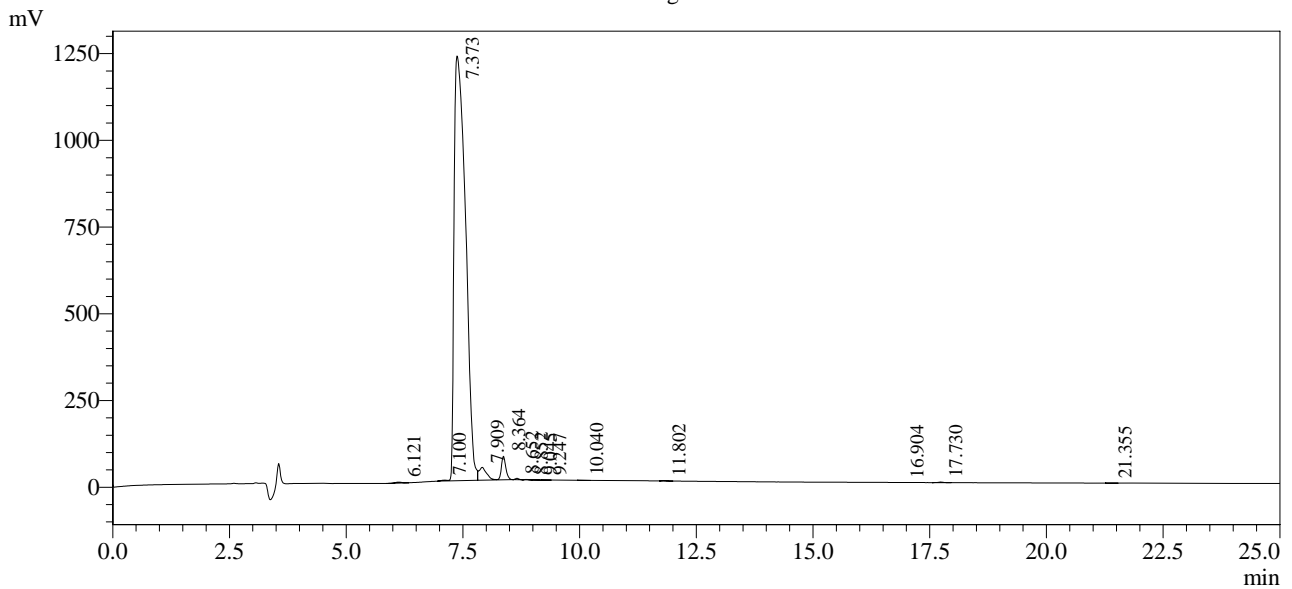

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.121	25705	2749	0.118
2	7.100	24223	2765	0.111
3	7.373	20766510	1224651	95.512
4	7.909	421996	37188	1.941
5	8.364	451852	68059	2.078
6	8.652	20828	3916	0.096
7	8.852	6942	1380	0.032
8	9.045	1767	318	0.008
9	9.247	1720	356	0.008
10	10.040	1105	174	0.005
11	11.802	5149	861	0.024
12	16.904	1192	112	0.005
13	17.730	11759	1597	0.054
14	21.355	1593	192	0.007
Total		21742343	1344318	100.000