

Sample Name : Rabies Virus Glycoprotein  
 Cat No. : RP20464  
 Lot No. : E4984719I  
 Time Processed : 4:45:59 PM  
 Month-Day-Year Processed : 09/29/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

### <Chromatogram>

mV

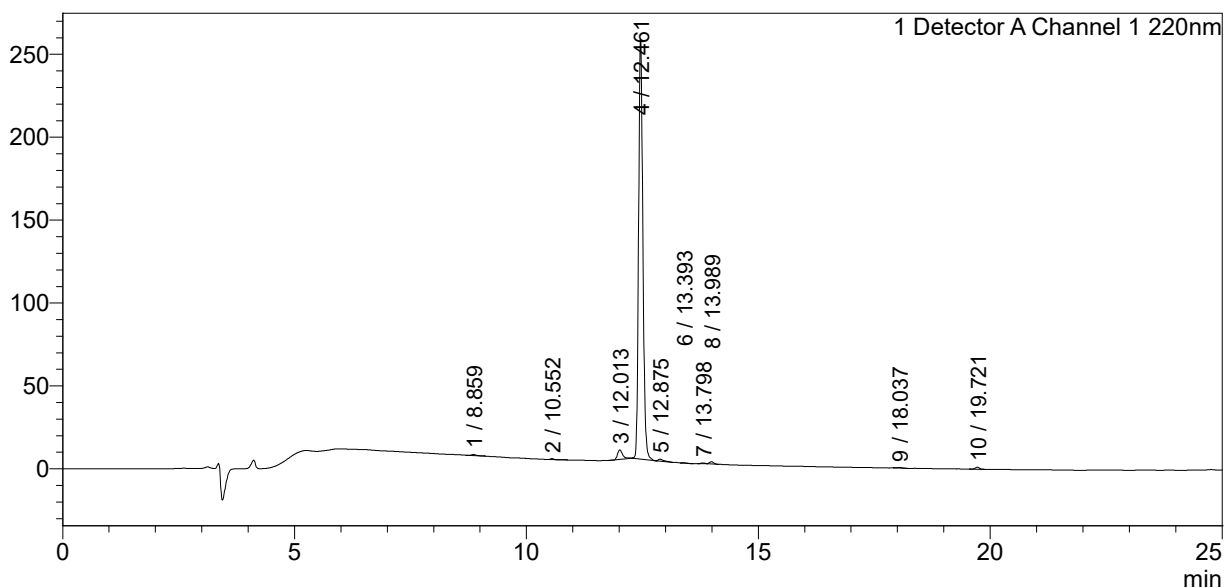

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.859	4283	684	0.253
2	10.552	3056	621	0.180
3	12.013	43807	5684	2.585
4	12.461	1611554	253319	95.095
5	12.875	10600	1241	0.625
6	13.393	1438	254	0.085
7	13.798	2603	481	0.154
8	13.989	7565	1285	0.446
9	18.037	2829	446	0.167
10	19.721	6936	1181	0.409
Total		1694672	265198	100.000