

Sample Name :Gastric Inhibitory Peptide (GIP), human  
 Cat No. :RP10795 :  
 Lot No. PE2561811  
 Time Processed :14:16:12  
 Month-Day-Year Processed :10/28/18

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ17010508

<Chromatogram>

mV

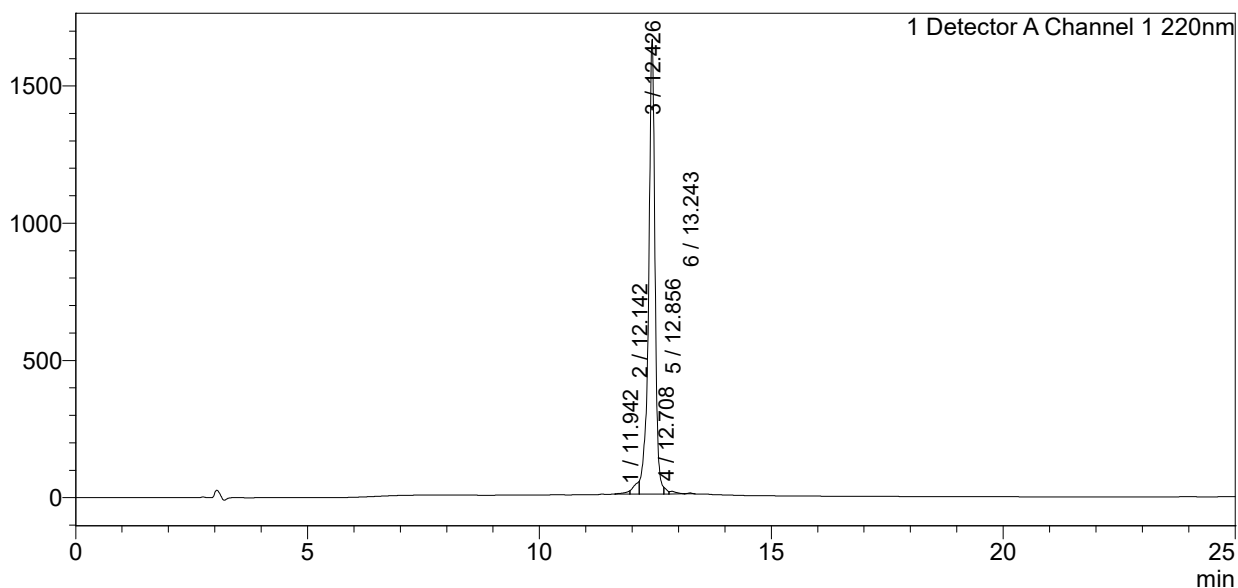

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.942	81018	10842	0.492
2	12.142	362550	44065	2.202
3	12.426	15795067	1657450	95.941
4	12.708	98887	20748	0.601
5	12.856	100801	9588	0.612
6	13.243	24913	3600	0.151
Total		16463235	1746293	100.000