


# Mass Spectrum

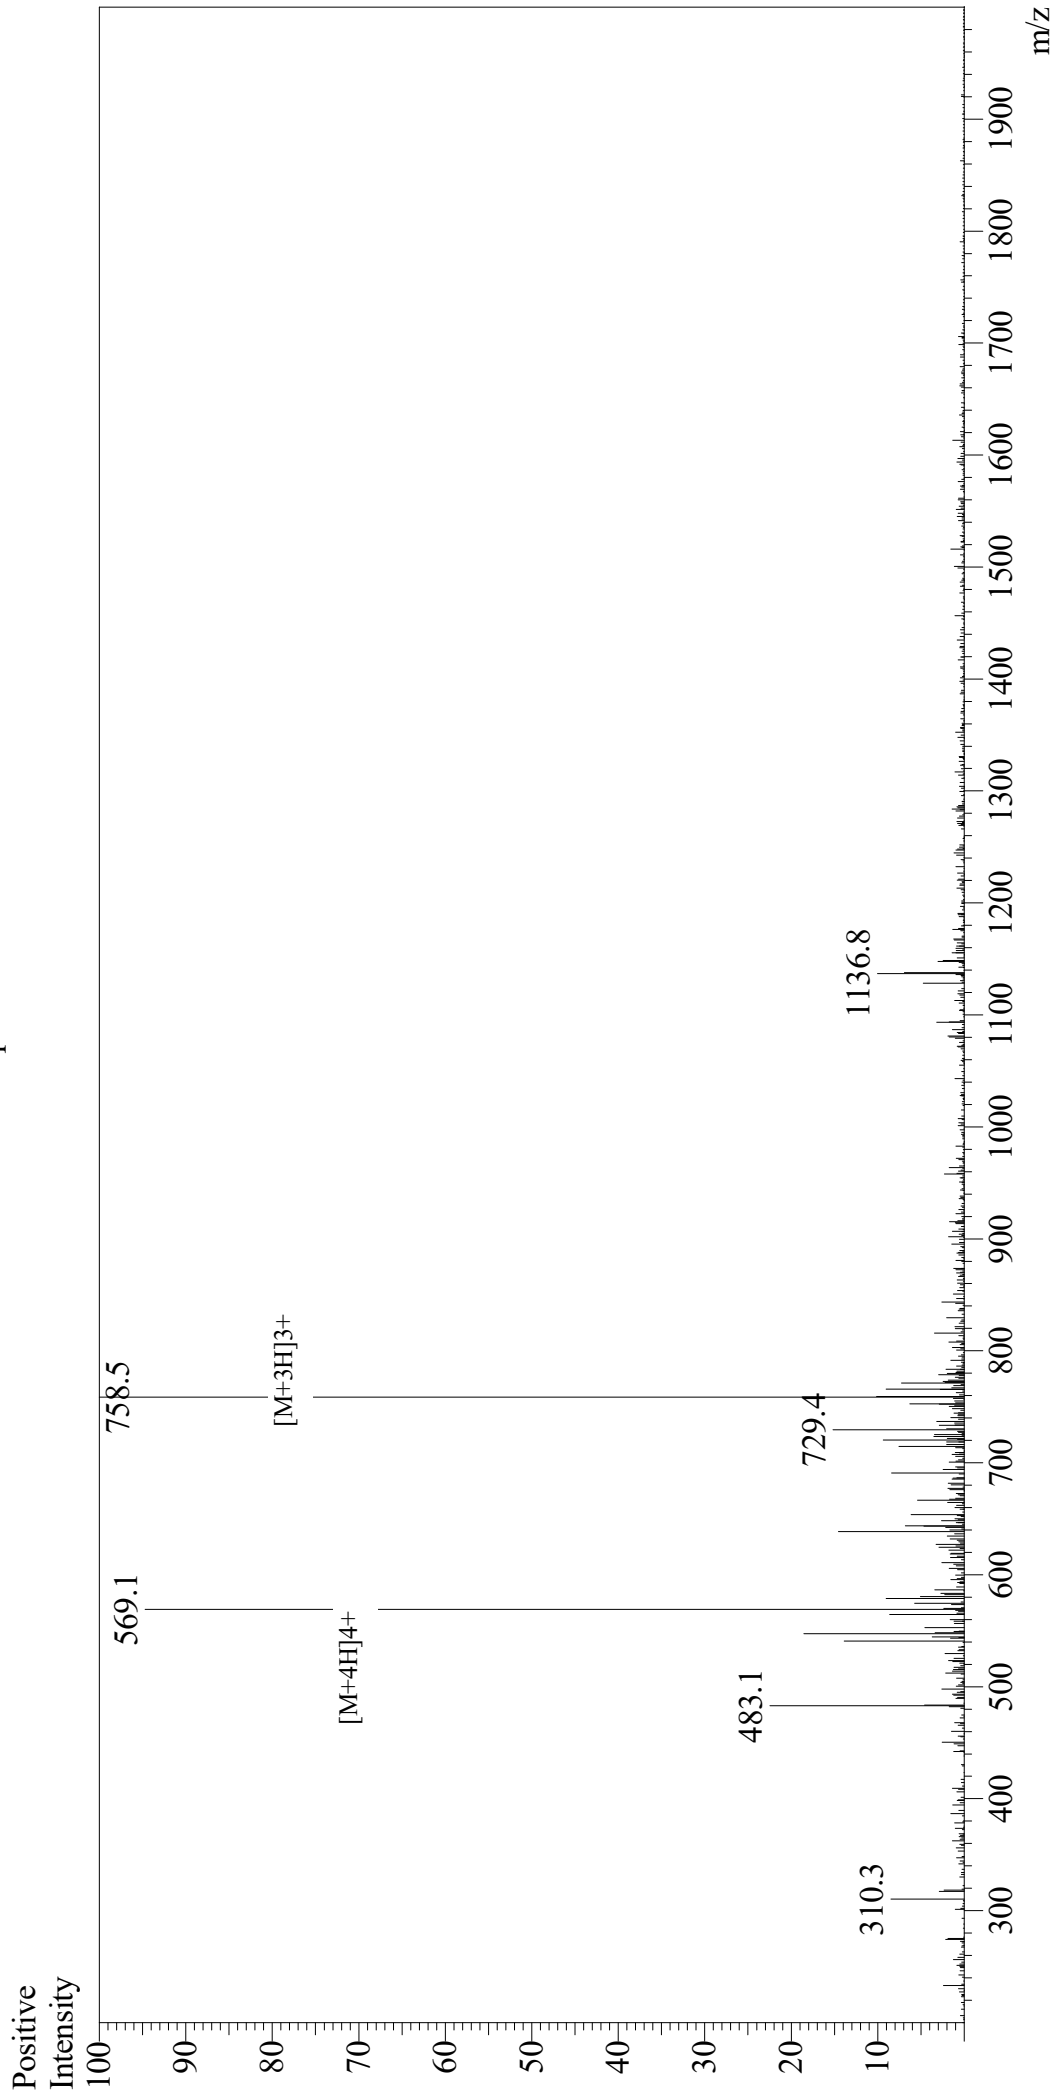

## Sample Information

User : Gary  
Month-Day Processed : 06/20/19  
Time Processed : 07:59:46 AM  
Injection Volume : 0.4  
Sample Name : Flagelin22  
Cat No. : RP19986  
Lot No. : E3923519F  
Theoretical MW : 2272.50  
Observed MW : 2272.5

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH