

Sample Name :OVA Peptide (257-264)
 Cat No. : RP10611
 Lot No. : E4701320K
 Time Processed : 8:26:46
 Month-Day-Year Processed : 11/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

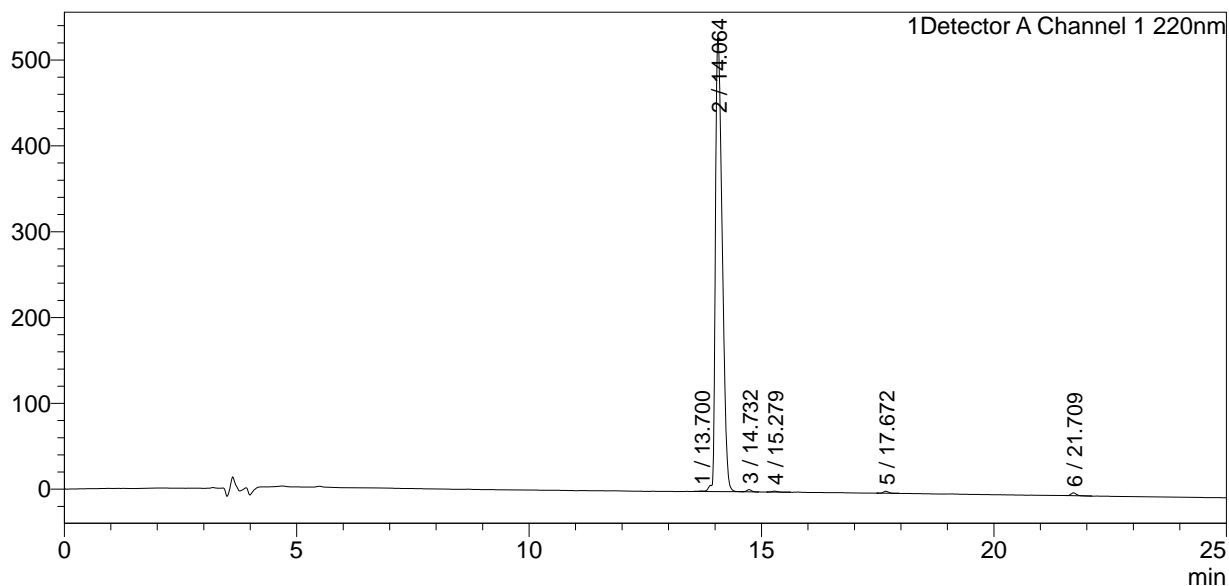

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.700	4424	580	0.081
2	14.064	5371948	528432	98.617
3	14.732	17880	2518	0.328
4	15.279	9337	1139	0.171
5	17.672	17324	2258	0.318
6	21.709	26393	3378	0.485
Total		5447306	538306	100.000