


Mass Spectrum

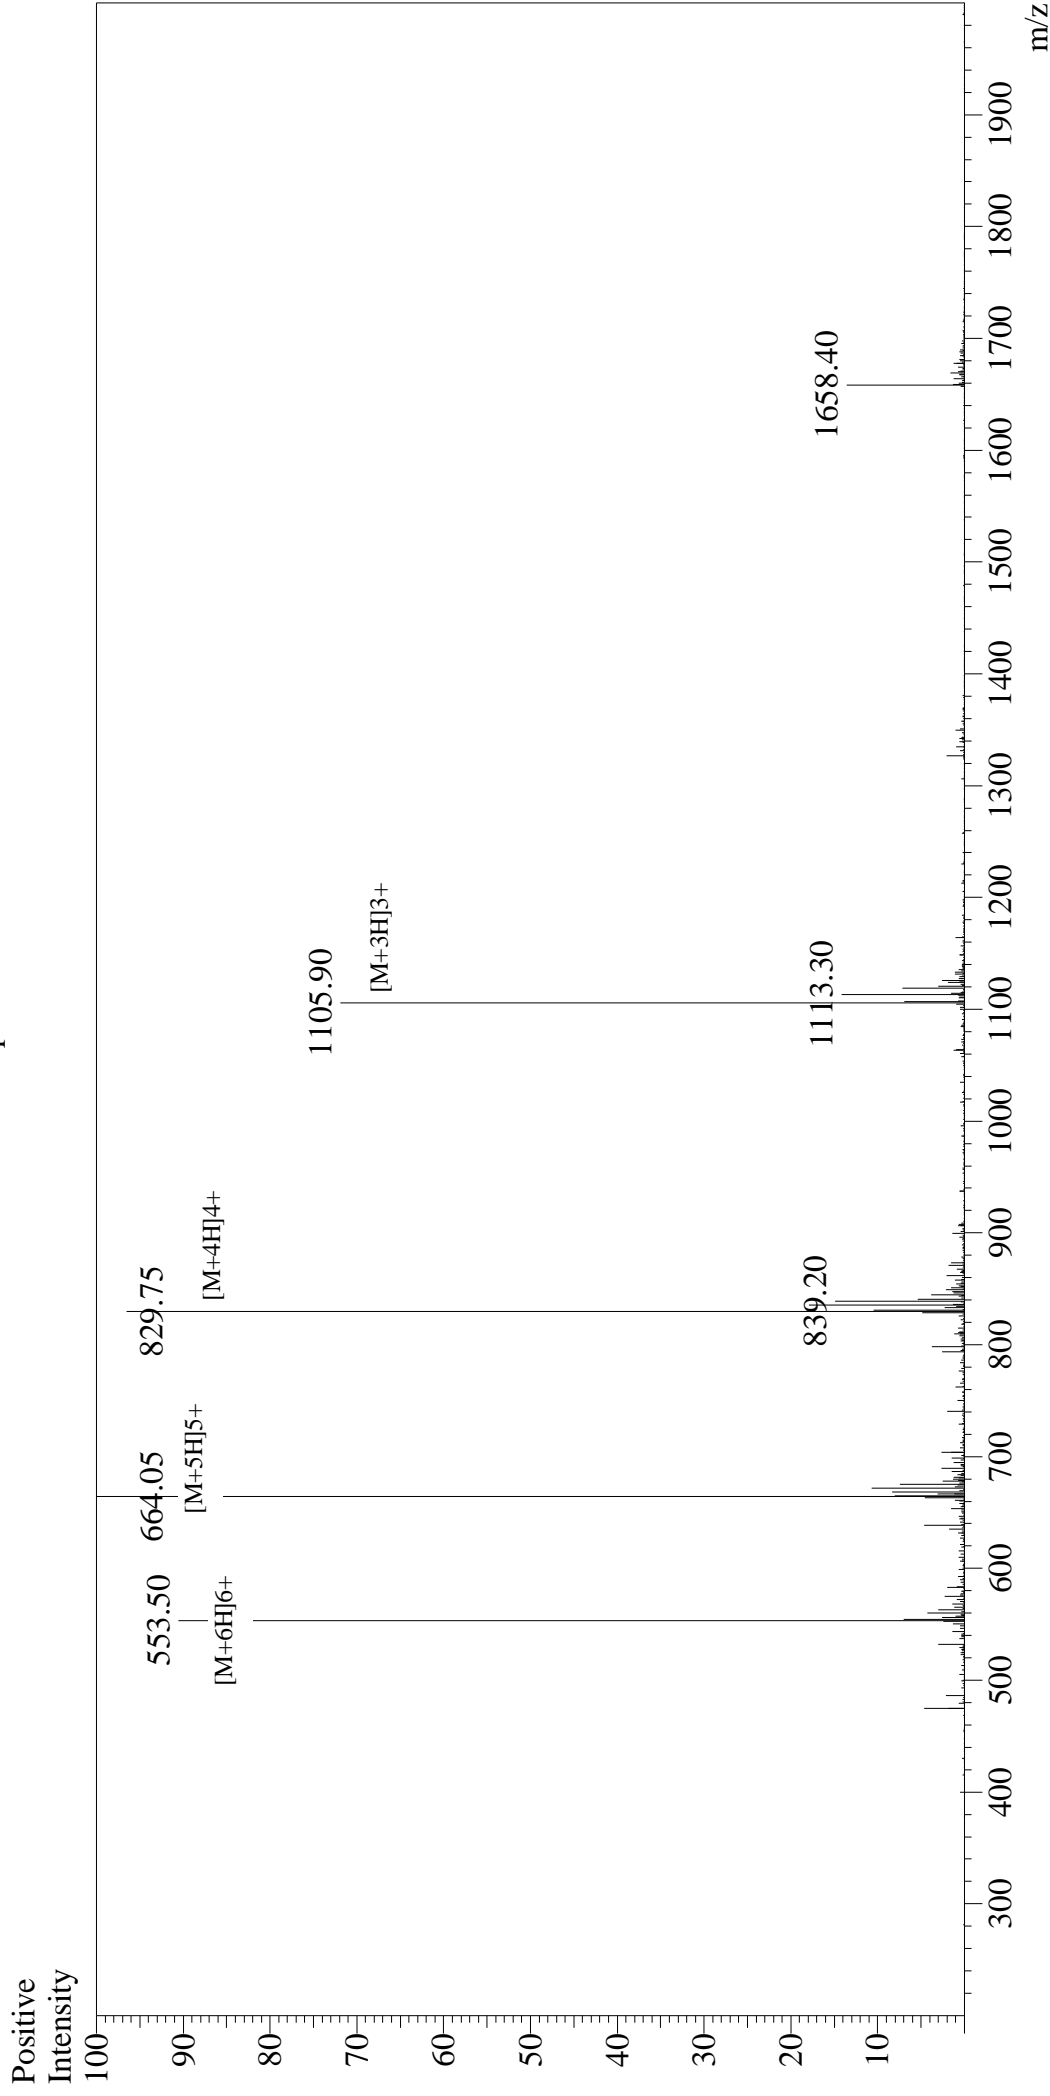

Sample Information

User : Gary
 Month-Day Processed : 06/08/17
 Time Processed : 16:20:33
 Injection Volume : 0.2
 Sample Name : Ghrelin_rat
 Cat No. : RPI0781
 Lot No. : PE6611706
 Theoretical MW : 3314.80
 Observed MW : 3315.25

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250°C
 Block Temp : 200°C

Interface Bias : +4.5kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2ml/min
 B.conc : 50%H2O/50%MeOH