


Mass Spectrum

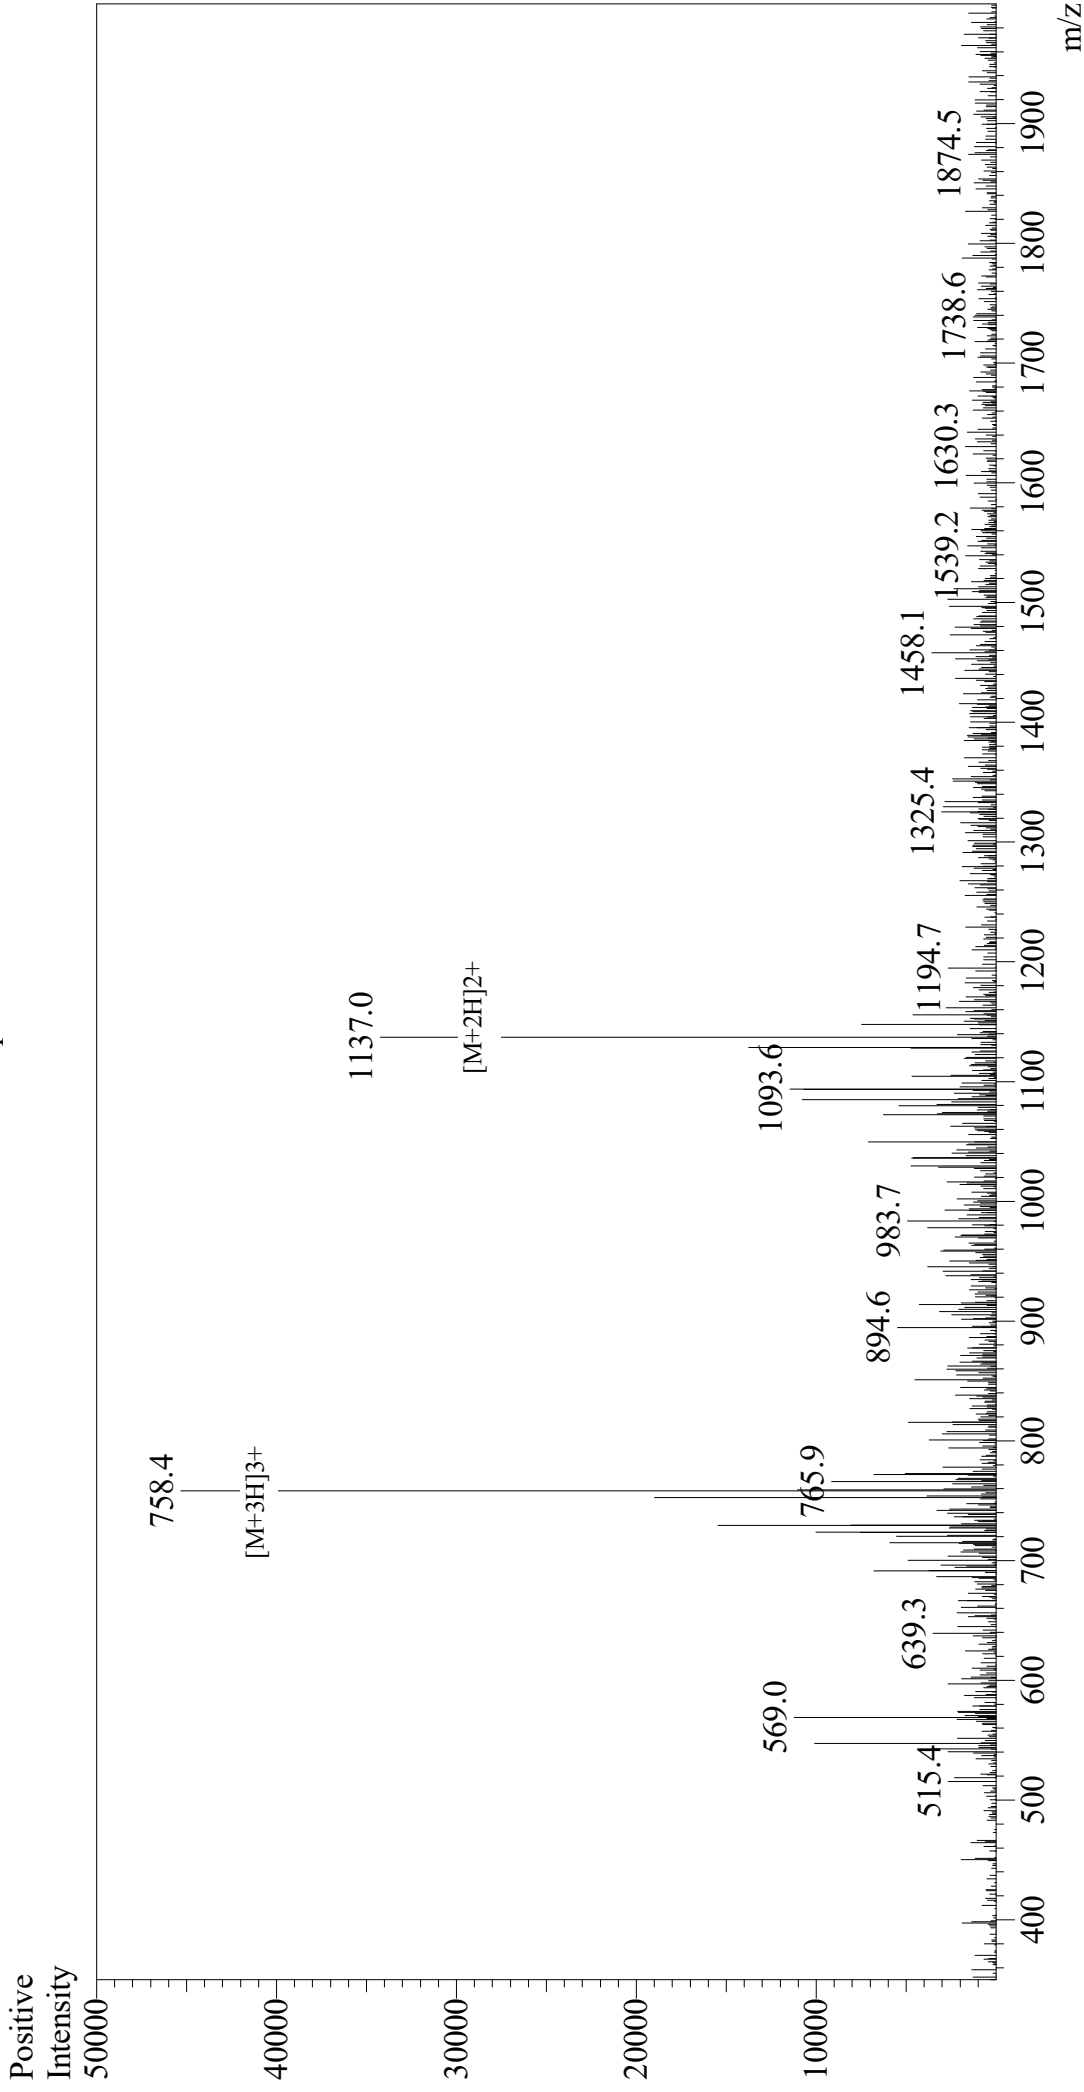

Sample Information
Month-Day Processed : 01/17/21
Time Processed : 10:08:16 AM
Injection Volume : 0.4
Sample Name : Flagelin22
Cat No : RP19986
Lot No : E4575521A
Theoretical MW : 2272.50
Observed MW : 2272.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H2O/50% MeOH