

Sample Name :hgp100(25-33)
 Cat No. :RP20344;
 Lot No. :PE1621904;
 Time Processed :8:58:17 PM
 Month-Day-Year Processed :04/06/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|-----------------|-------|
| 0.01 | Pumps | Solvent B Conc. | 5 |
| 25.00 | Pumps | Solvent B Conc. | 65 |
| 25.01 | Pumps | Solvent B Conc. | 95 |
| 27.00 | Pumps | Solvent B Conc. | 95 |
| 27.01 | Pumps | Solvent B Conc. | 5 |
| 35.00 | Pumps | Solvent B Conc. | 5 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

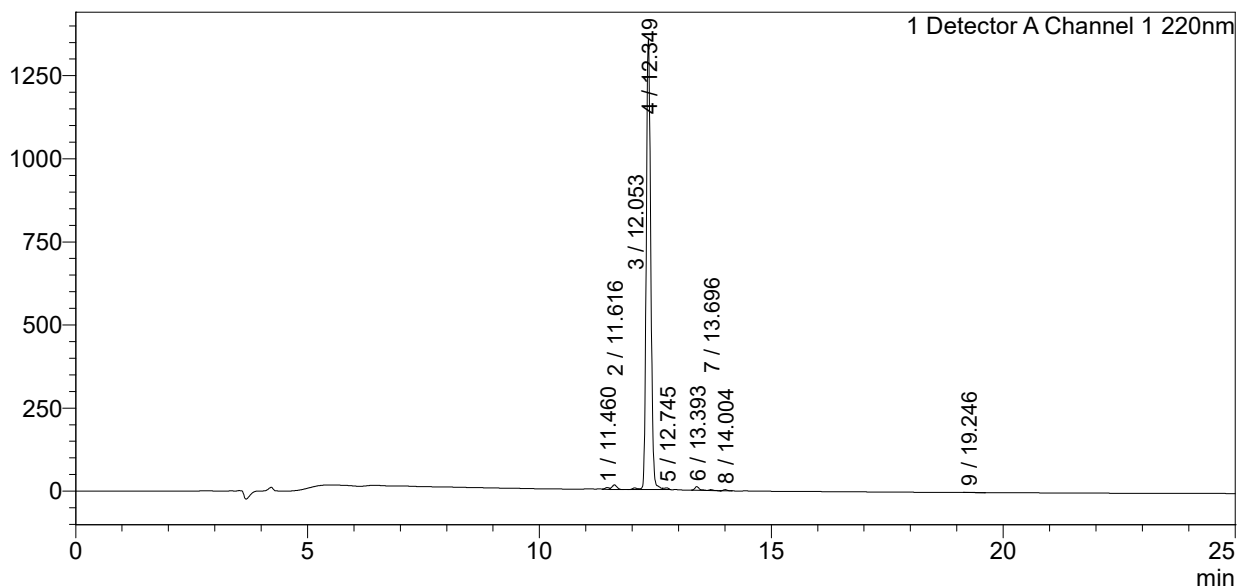

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|---------|---------|
| 1 | 11.460 | 33465 | 5375 | 0.354 |
| 2 | 11.616 | 97851 | 13869 | 1.034 |
| 3 | 12.053 | 34172 | 4982 | 0.361 |
| 4 | 12.349 | 9148856 | 1358478 | 96.709 |
| 5 | 12.745 | 31661 | 4615 | 0.335 |
| 6 | 13.393 | 76057 | 11260 | 0.804 |
| 7 | 13.696 | 15497 | 2616 | 0.164 |
| 8 | 14.004 | 20648 | 3632 | 0.218 |
| 9 | 19.246 | 2012 | 99 | 0.021 |
| Total | | 9460219 | 1404926 | 100.000 |