

Sample Name :C-Myc Peptide
 Cat. No. : RP11731
 Lot. No. :E8603320A
 Time Processed :10:08:22
 Month-Day-Year Processed :01/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

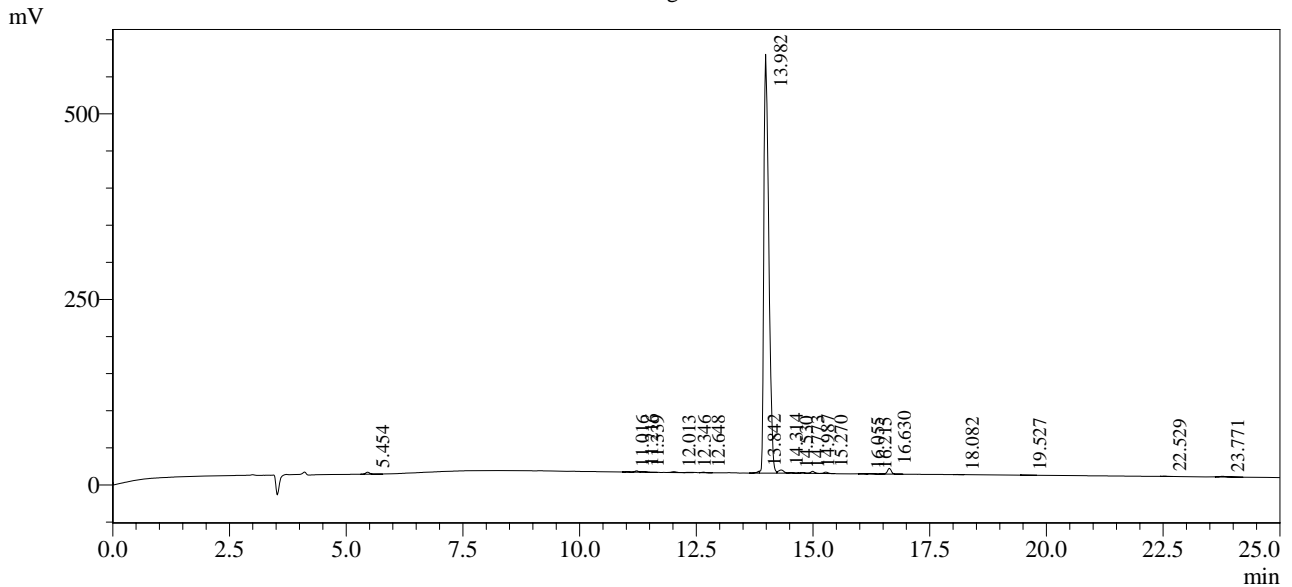

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.454	15898	2622	0.362
2	11.016	2357	313	0.054
3	11.216	10144	1714	0.231
4	11.339	6548	690	0.149
5	12.013	7621	1121	0.174
6	12.346	3124	518	0.071
7	12.648	3727	683	0.085
8	13.842	10815	2639	0.246
9	13.982	4192537	564439	95.468
10	14.314	34200	4231	0.779
11	14.530	4245	698	0.097
12	14.773	6712	1058	0.153
13	14.987	15552	2653	0.354
14	15.270	11569	1863	0.263
15	16.055	1183	239	0.027
16	16.215	3661	447	0.083
17	16.630	45290	7811	1.031
18	18.082	1267	205	0.029
19	19.527	1123	94	0.026
20	22.529	2396	348	0.055
21	23.771	11585	959	0.264
Total		4391555	595345	100.000