

Sample Name : Hexa-His
 Cat. No. : RP11737
 Lot. No. : PE2461707

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	0	
5.00	Pumps	Pump B Conc.	0	
20.00	Pumps	Pump B Conc.	30	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	0	
40.00	Pumps	Pump B Conc.	0	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

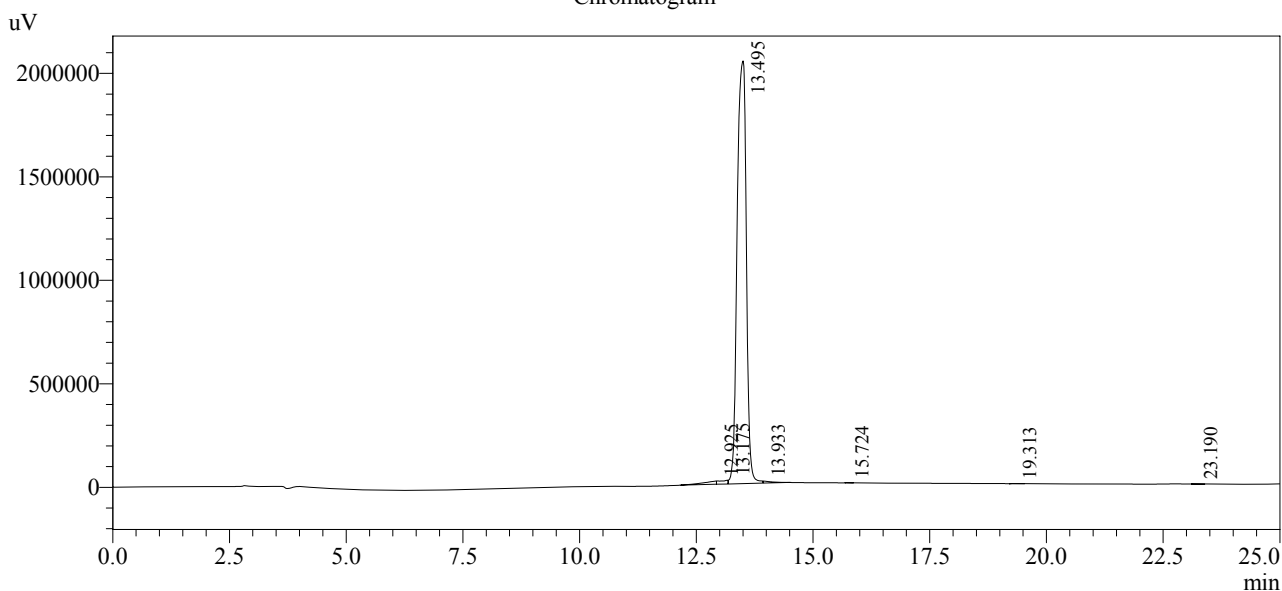

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.925	317615	15877	1.114
2	13.175	238143	18217	0.835
3	13.495	27829444	2043041	97.574
4	13.933	126053	9945	0.442
5	15.724	1376	256	0.005
6	19.313	4948	637	0.017
7	23.190	3885	551	0.014
Total		28521465	2088524	100.000