

Sample Name :Melittin,honey bee
 Cat No. :RP20415
 Lot No. :E7109421A
 Time Processed :8:46:22
 Month-Day-Year Processed :01/16/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

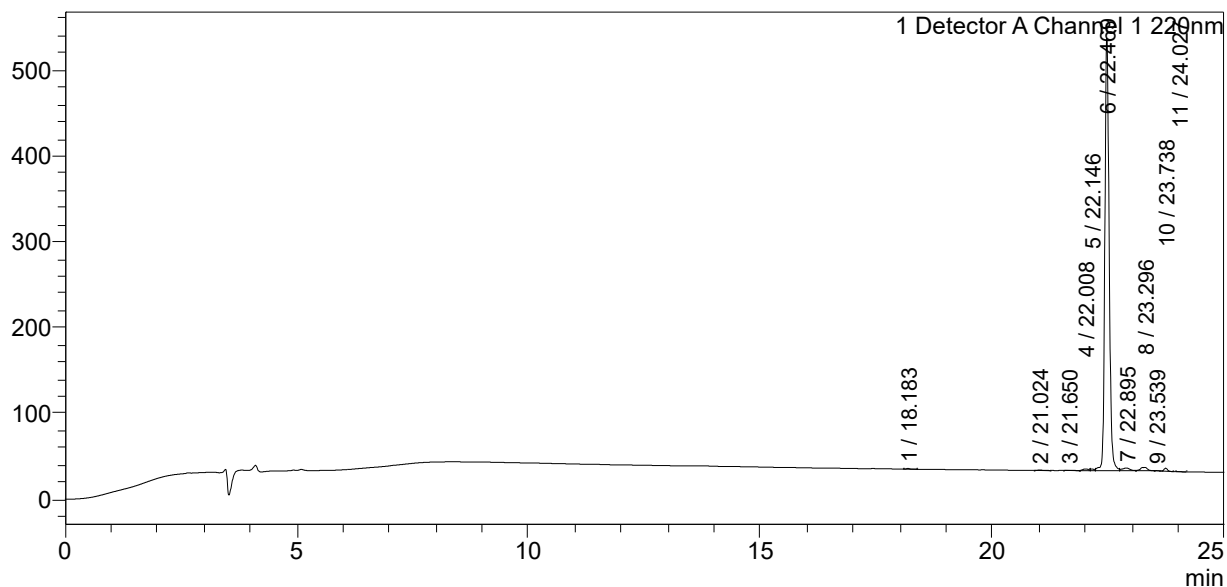

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	18.183	4132	782	0.122
2	21.024	3388	524	0.100
3	21.650	2883	345	0.085
4	22.008	16211	1913	0.480
5	22.146	11945	1867	0.353
6	22.469	3244346	504231	95.968
7	22.895	33996	3121	1.006
8	23.296	41714	3889	1.234
9	23.539	2262	460	0.067
10	23.738	18404	3543	0.544
11	24.027	1362	286	0.040
Total		3380645	520961	100.000