

Sample Name :mTRP-2(180-188)  
 Cat No. :RP20250  
 Lot No. :E6784021E  
 Time Processed :3:07:53 PM  
 Month-Day-Year Processed :05/26/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010324

<Chromatogram>

mV

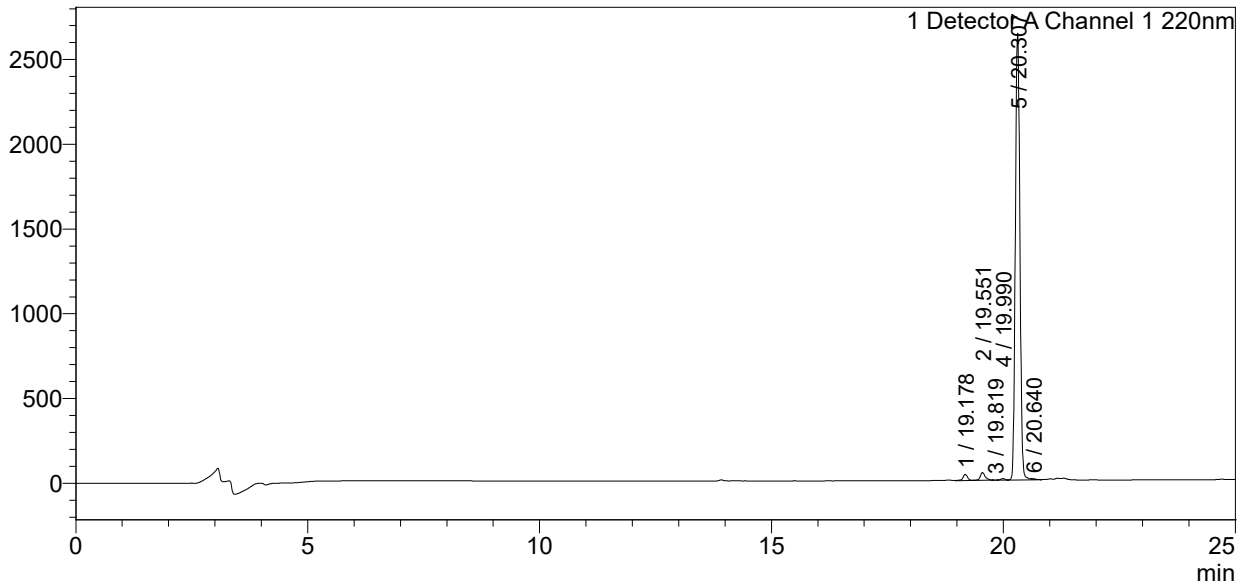

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	19.178	247424	35788	1.322
2	19.551	342924	46153	1.833
3	19.819	5987	1173	0.032
4	19.990	52829	8605	0.282
5	20.307	18051814	2636486	96.473
6	20.640	10722	2704	0.057
Total		18711699	2730909	100.000