

Sample Name :LAH4  
 Cat. No. : RP20096  
 Lot. No. : PE4341809  
 Time Processed : 15:21:10  
 Month-Day-Year Processed : 10/06/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
95.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

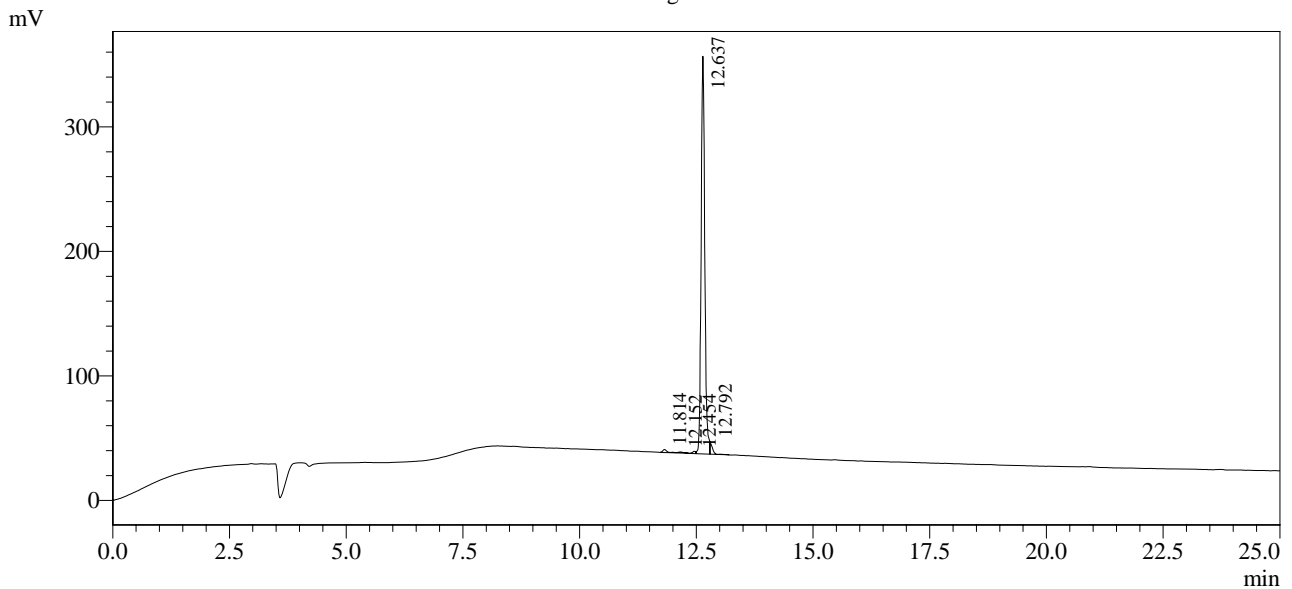

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.814	15800	2375	0.876
2	12.152	8932	881	0.495
3	12.454	8387	1772	0.465
4	12.637	1738491	319344	96.349
5	12.792	32750	10296	1.815
Total		1804360	334667	100.000