

Sample Name : PACAP-Related Peptide (PRP), human
 Cat. No. : RP10341
 Lot. No. : E4700419I
 Time Processed : 15:09:35
 Month-Day-Year Processed : 09/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	35	
25.00	Pumps	Pump A B.Conc	95	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	35	
35.00	Pumps	Pump A B.Conc	35	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

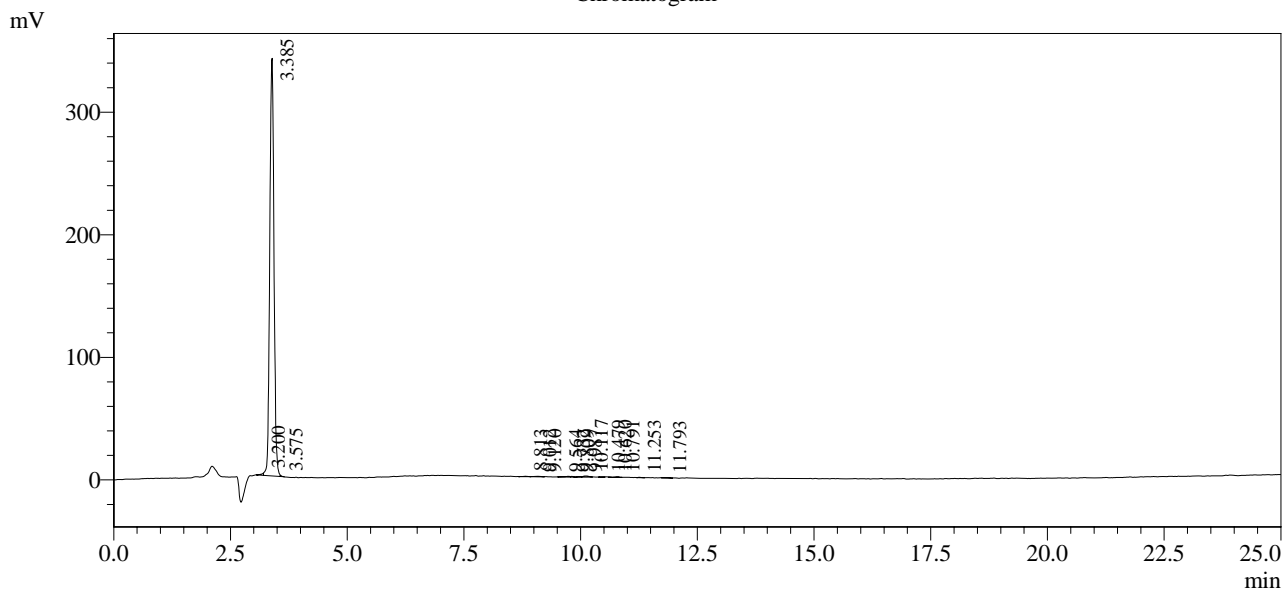

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	3.200	6166	1666	0.284
2	3.385	2129383	340768	98.061
3	3.575	1551	957	0.071
4	8.813	2561	359	0.118
5	9.012	2406	304	0.111
6	9.120	1303	303	0.060
7	9.564	1011	243	0.047
8	9.732	4486	614	0.207
9	9.809	2073	559	0.095
10	9.987	2677	423	0.123
11	10.117	8471	981	0.390
12	10.479	1938	320	0.089
13	10.620	1066	266	0.049
14	10.791	2405	477	0.111
15	11.253	1250	263	0.058
16	11.793	2735	350	0.126
Total		2171483	348853	100.000