

Sample Name :DYKDDDDK Peptide  
 Cat No. : RP10586  
 Lot No. : E4744219I  
 Time Processed : 13:01:23  
 Month-Day-Year Processed : 09/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	0
5.00	Pumps	Pump B Conc.	0
20.00	Pumps	Pump B Conc.	30
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
31.00	Pumps	Pump B Conc.	95
31.01	Pumps	Pump B Conc.	0
40.00	Pumps	Pump B Conc.	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

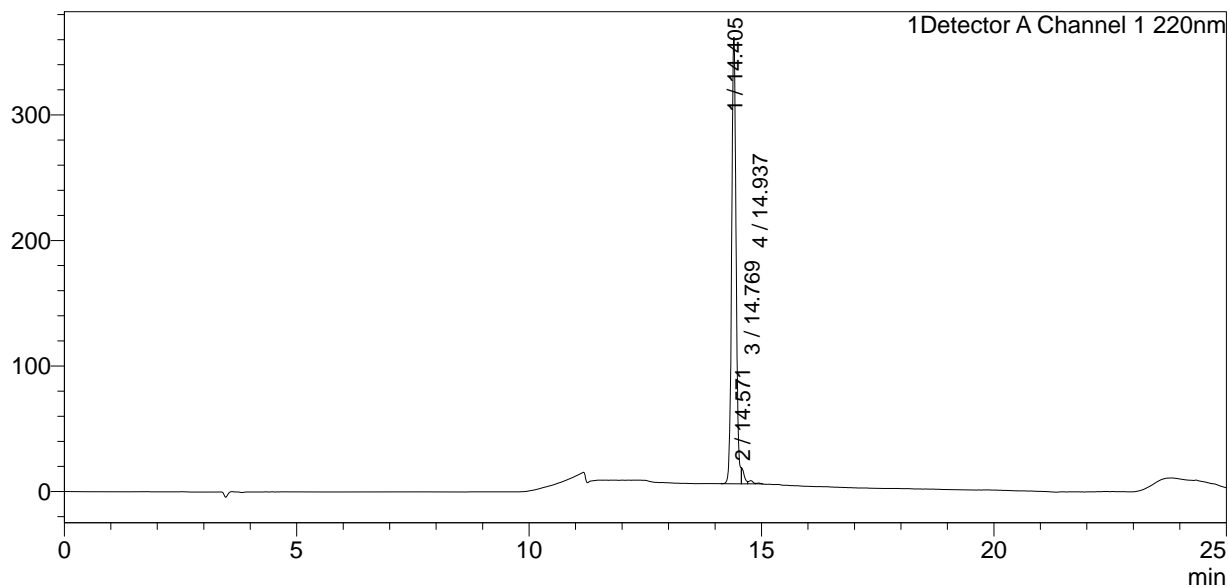

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.405	2357918	355643	97.054
2	14.571	51175	12834	2.106
3	14.769	16772	2530	0.690
4	14.937	3620	661	0.149
Total		2429485	371668	100.000