

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :E8361021F
 Time Processed :8:00:14 AM
 Month-Day-Year Processed :06/29/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

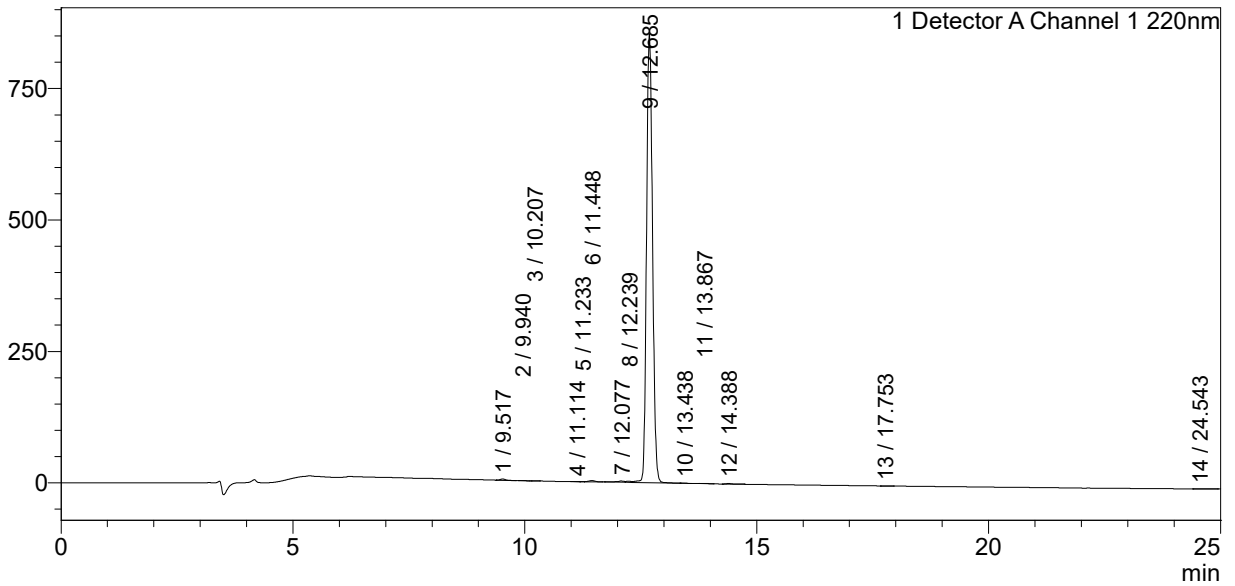

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.517	19819	2396	0.256
2	9.940	1582	239	0.020
3	10.207	1258	224	0.016
4	11.114	4615	458	0.060
5	11.233	3072	519	0.040
6	11.448	23868	2378	0.308
7	12.077	28362	2410	0.366
8	12.239	17317	2085	0.224
9	12.685	7619044	854493	98.445
10	13.438	2626	420	0.034
11	13.867	4889	558	0.063
12	14.388	8783	1088	0.113
13	17.753	1325	143	0.017
14	24.543	2869	117	0.037

Peak#	Ret. Time	Area	Height	Area%
Total		7739428	867526	100.000