

Sample Name :DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : PE1581802

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

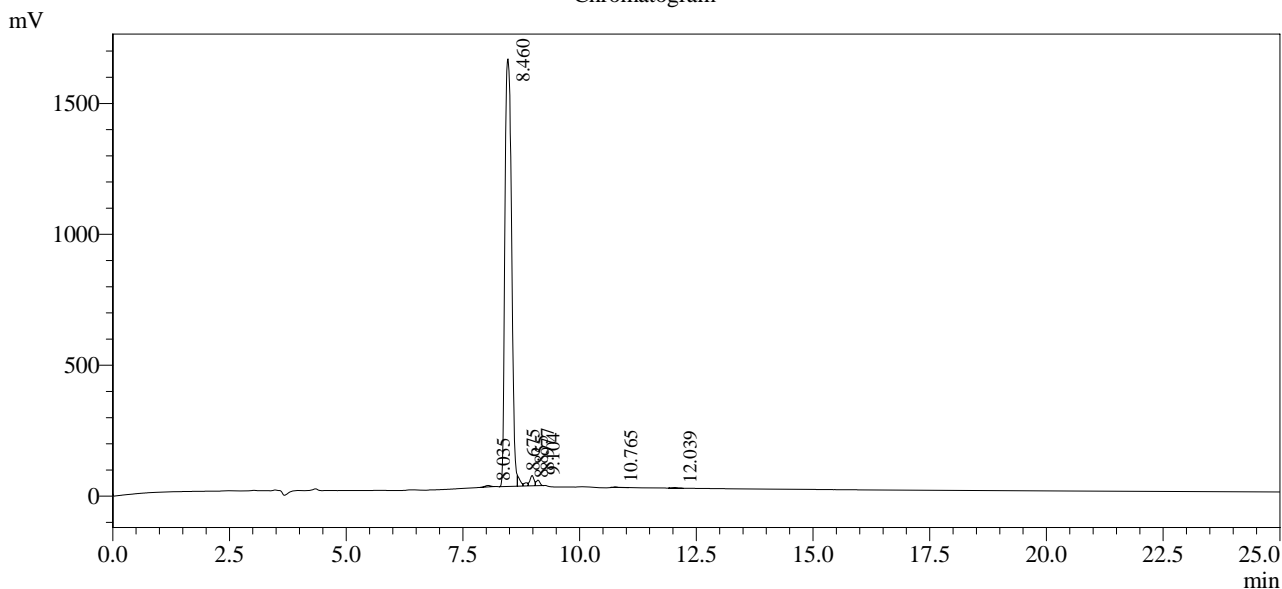

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.035	46277	5720	0.276
2	8.460	16153936	1633382	96.177
3	8.675	150333	38776	0.895
4	8.855	75973	12217	0.452
5	8.977	233069	39297	1.388
6	9.104	115684	21191	0.689
7	10.765	13134	2166	0.078
8	12.039	7667	1271	0.046
Total		16796072	1754021	100.000