

Sample Name :Parathyroid Hormone(PTH)(1-34),Human  
 Cat. No. : RP01001  
 Lot. No. : PE9361901  
 Time Processed :7:23:40  
 Month-Day-Year Processed : 01/09/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

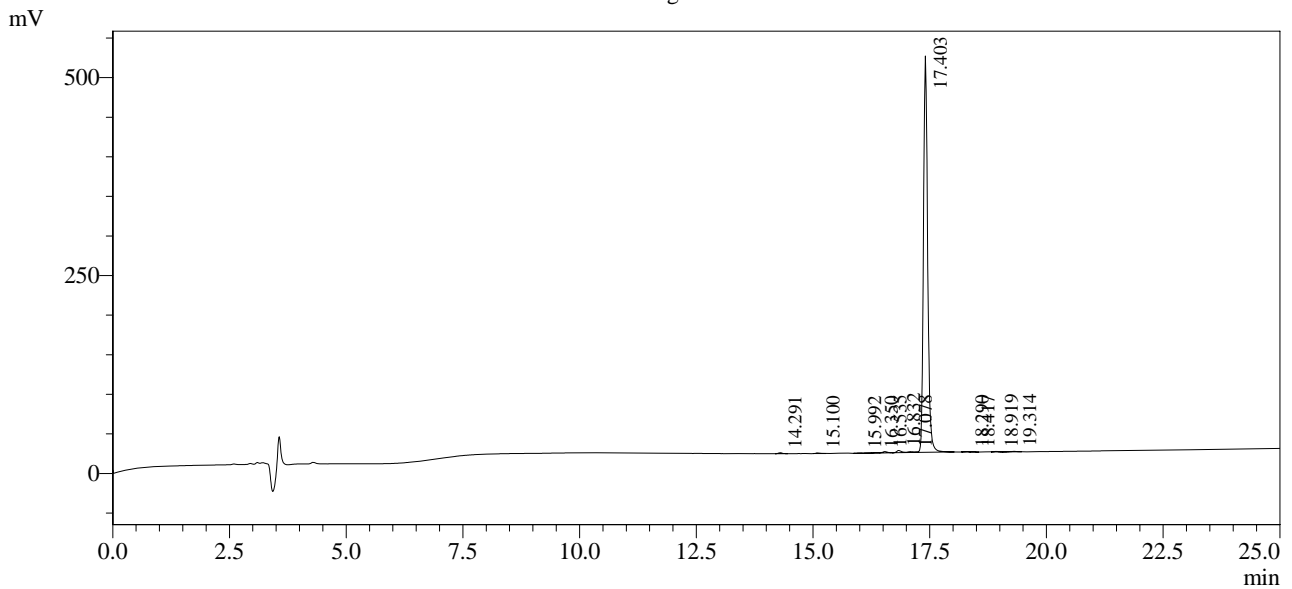

1 Det. A Ch1 / 220nm  
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.291	7056	1266	0.219
2	15.100	4986	880	0.155
3	15.992	2100	220	0.065
4	16.350	2982	357	0.092
5	16.535	12414	1682	0.385
6	16.832	20644	2843	0.640
7	17.078	11185	1117	0.347
8	17.403	3148738	500676	97.665
9	18.290	2175	421	0.067
10	18.417	1800	330	0.056
11	18.919	3982	669	0.124
12	19.314	5947	682	0.184
Total		3224009	511143	100.000