

Sample Name : OVA Peptide(257-264)
 Cat. No. : RP10611
 Lot. No. : PE0081701

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

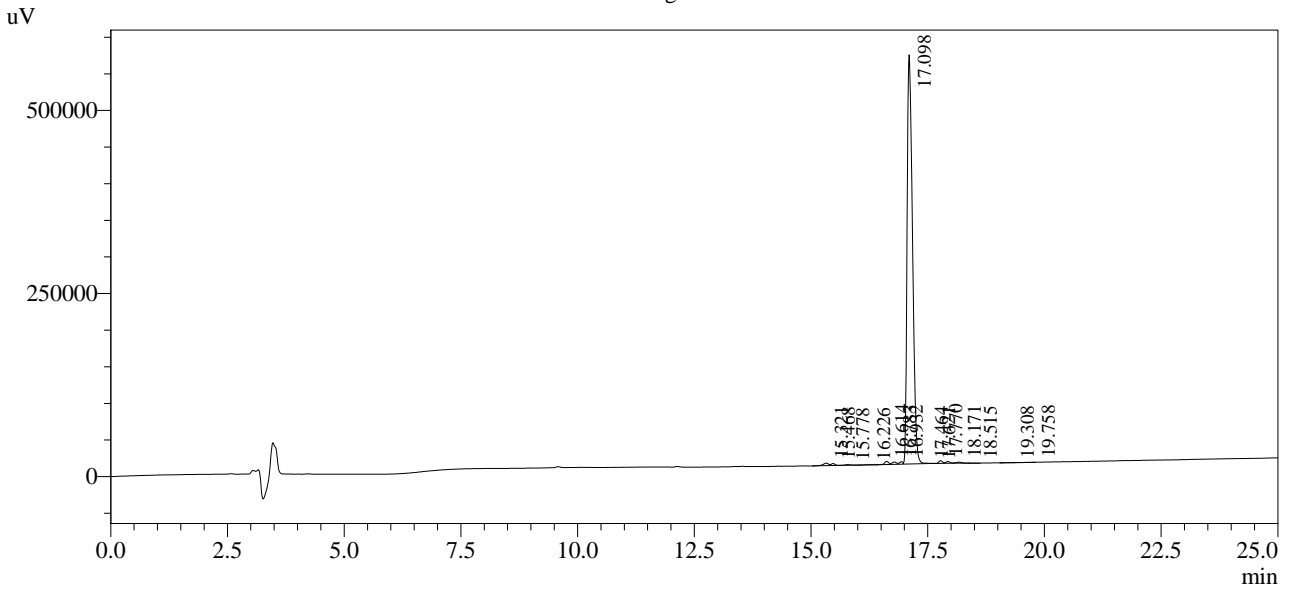

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.321	28782	3408	0.617
2	15.468	16008	2743	0.343
3	15.778	9740	1068	0.209
4	16.226	3144	319	0.067
5	16.614	27543	4262	0.590
6	16.783	21246	3229	0.455
7	16.932	17601	3446	0.377
8	17.098	4491929	558815	96.228
9	17.464	4818	727	0.103
10	17.621	829	177	0.018
11	17.770	32586	3559	0.698
12	18.171	10707	1238	0.229
13	18.515	672	103	0.014
14	19.308	1038	61	0.022
15	19.758	1373	45	0.029
Total		4668017	583200	100.000