

Sample Name : HA-peptide  
 Cat. No. : RP11735  
 Lot. No. : PE4951802

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

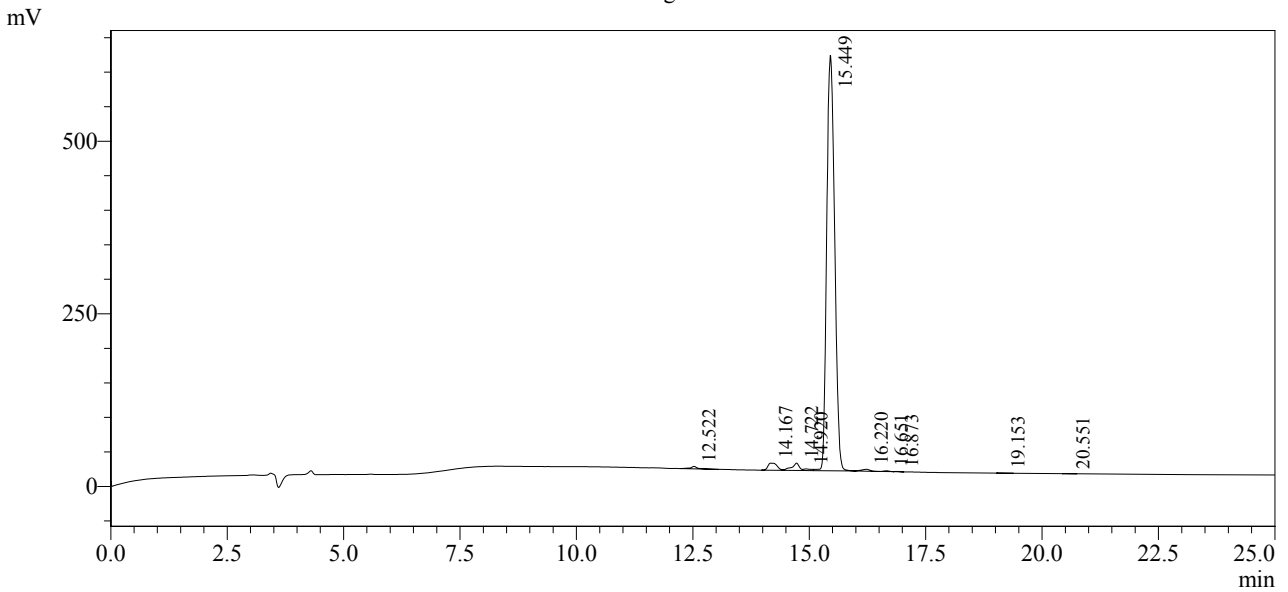

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.522	36864	3487	0.492
2	14.167	139462	10229	1.861
3	14.722	116388	10599	1.553
4	14.920	26844	2293	0.358
5	15.449	7122637	601585	95.051
6	16.220	35225	2915	0.470
7	16.651	10215	1242	0.136
8	16.873	2978	446	0.040
9	19.153	1833	193	0.024
10	20.551	1069	133	0.014
Total		7493514	633123	100.000