

Sample Name :RGD  
 Cat. No. : RP20297  
 Lot. No. : E7490219H  
 Time Processed :10:03:52 AM  
 Month-Day-Year  
 Processed :09/04/2019  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010508

<Chromatogram>

mV

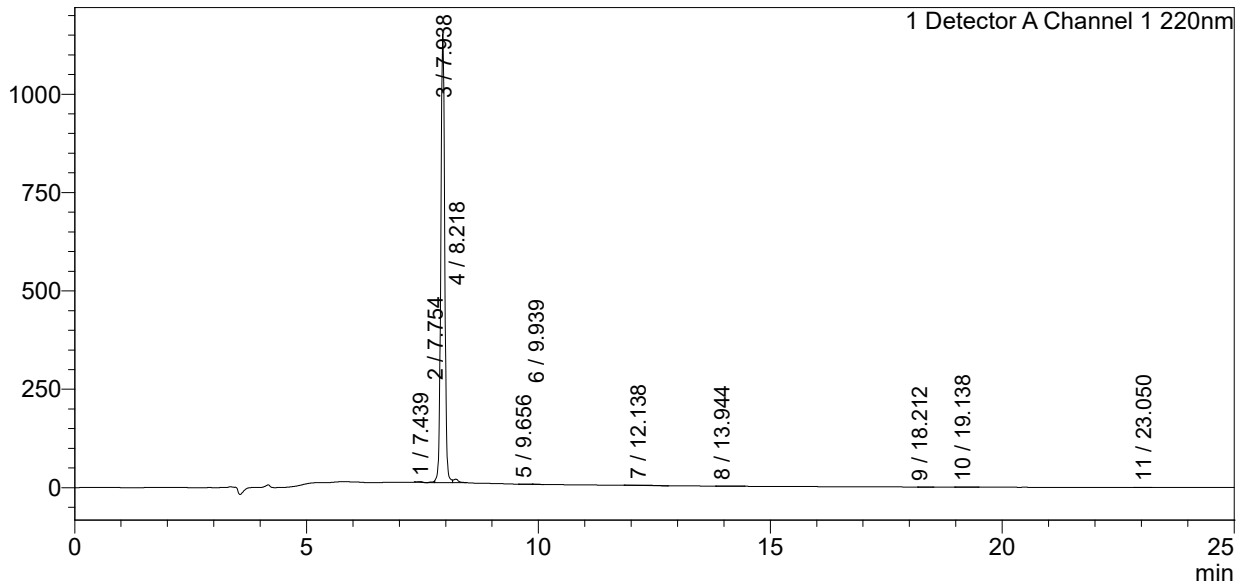

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.439	14798	2047	0.218
2	7.754	16198	3541	0.238
3	7.938	6672554	1141822	98.090
4	8.218	62678	8783	0.921
5	9.656	1024	90	0.015
6	9.939	2396	351	0.035
7	12.138	25771	679	0.379
8	13.944	2868	195	0.042
9	18.212	1536	135	0.023
10	19.138	1568	108	0.023
11	23.050	1080	91	0.016
Total		6802473	1157841	100.000