

Sample Name :OVA Peptide (257-264)
 Cat. No. : RP10611
 Lot. No. : E8070621C
 Time Processed :9:54:02
 Month-Day-Year Processed :03/11/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ20010140

<Chromatogram>

mV

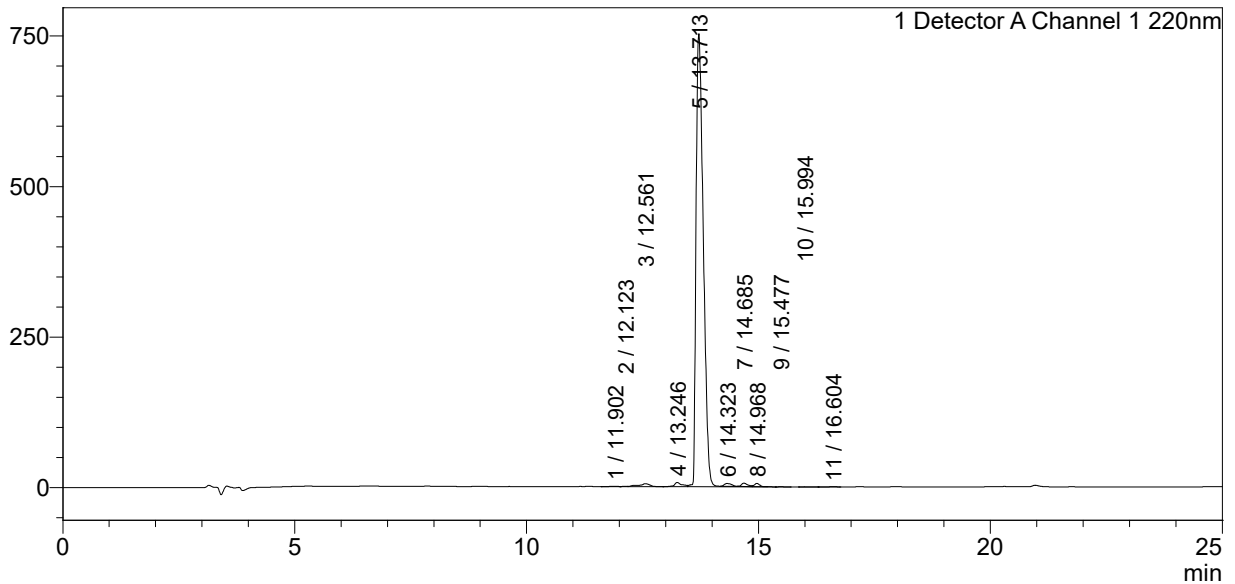

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.902	8215	791	0.097
2	12.123	5304	744	0.062
3	12.561	87264	5043	1.028
4	13.246	83838	7227	0.988
5	13.713	8150018	752777	96.029
6	14.323	51610	4681	0.608
7	14.685	52579	5638	0.620
8	14.968	40451	5394	0.477
9	15.477	1051	132	0.012
10	15.994	2007	156	0.024
11	16.604	4708	440	0.055
Total		8487045	783023	100.000