

Sample Name :GLP-1 (7-36), amide, human
 Cat. No. :RP10773
 Lot. No. :PE0491810
 Time Processed :12:44:48
 Month-Day-Year Processed :10/24/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

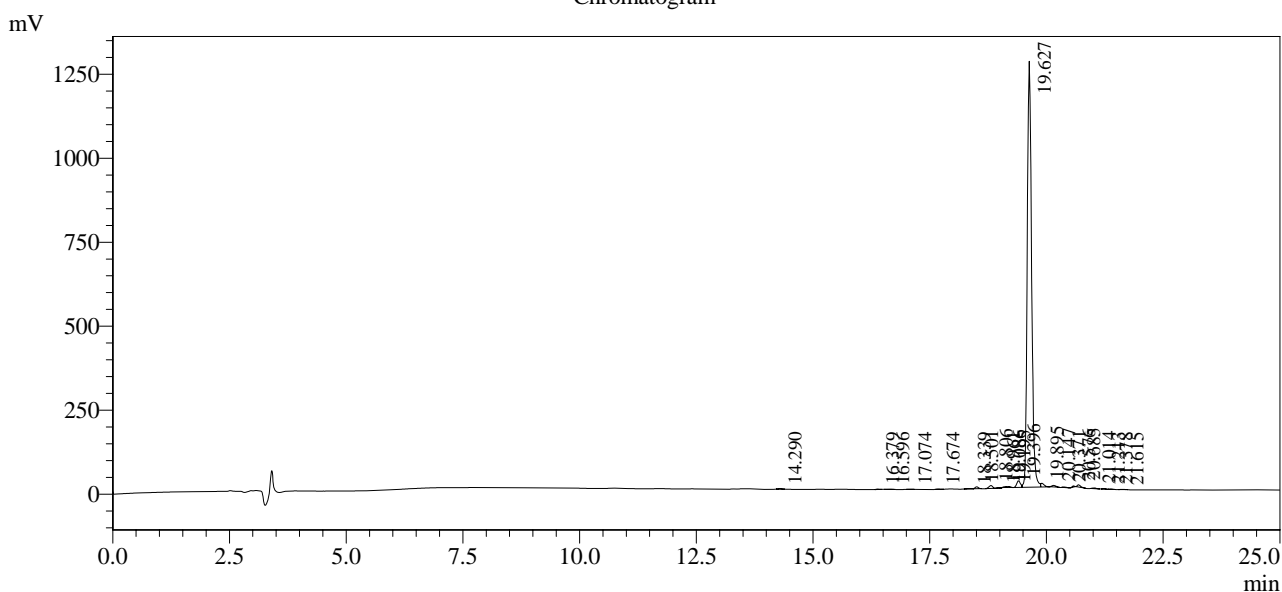

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.290	6771	1489	0.079
2	16.379	4877	1175	0.057
3	16.596	5592	1024	0.065
4	17.074	2338	476	0.027
5	17.674	4002	929	0.047
6	18.339	2535	490	0.030
7	18.501	26421	5527	0.308
8	18.806	47481	8431	0.553
9	18.961	3625	1058	0.042
10	19.086	6746	1799	0.079
11	19.195	7373	2188	0.086
12	19.396	108608	19575	1.265
13	19.627	8207418	1267347	95.562
14	19.895	51152	10855	0.596
15	20.147	28097	4429	0.327
16	20.371	7944	1347	0.092
17	20.576	13616	3625	0.159
18	20.685	32342	6780	0.377
19	21.014	10976	2052	0.128
20	21.213	2658	630	0.031
21	21.378	3748	932	0.044
22	21.615	4289	729	0.050
Total		8588610	1342887	100.000