

Sample Name :LL37 (Human)
 Cat.No :RP13323
 Lot.No : E5982120C
 Time Processed: 10:44:22
 Year-Month-Day: 2020/3/27

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010015

<Chromatogram>

mV

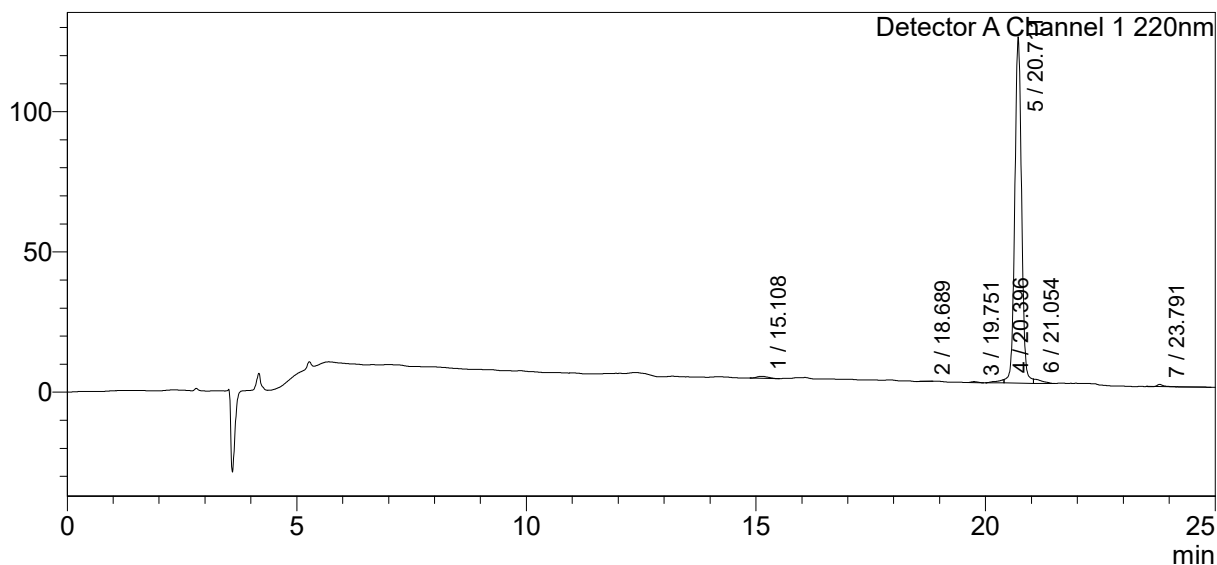

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.108	12157	722	0.910
2	18.689	1042	98	0.078
3	19.751	3735	361	0.280
4	20.396	12565	1168	0.941
5	20.711	1280756	123478	95.887
6	21.054	19053	1485	1.426
7	23.791	6386	782	0.478
Total		1335694	128093	100.000