

Sample Name :OVA G4 peptide  
 Cat. No. : RP20398  
 Lot. No. : PE6201708

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

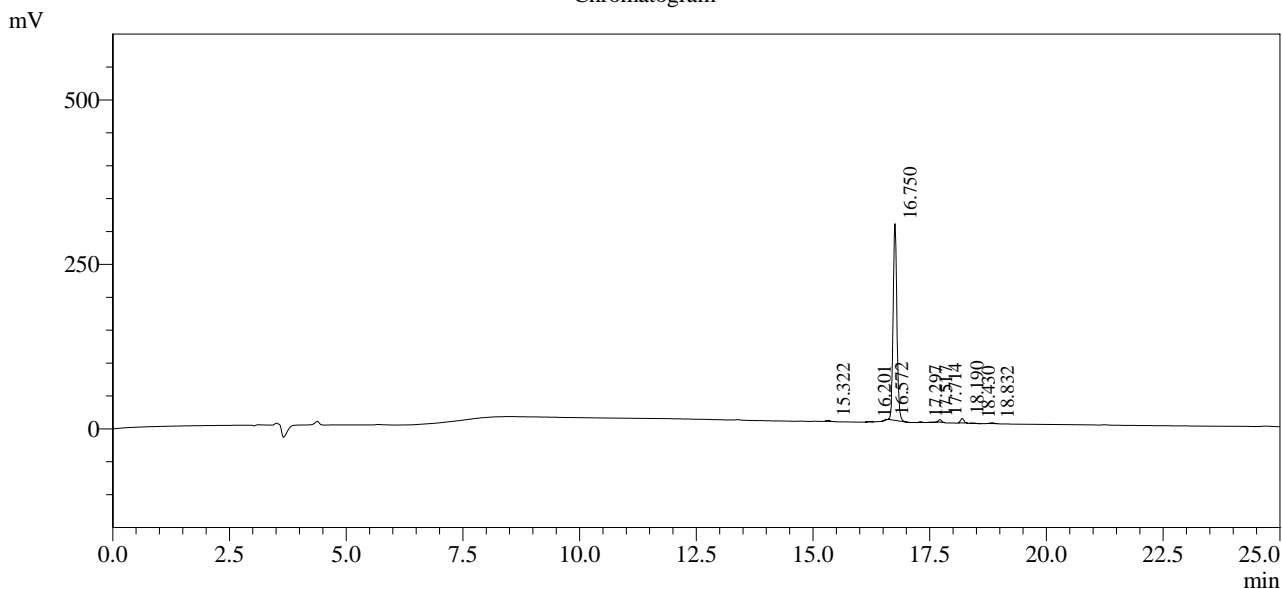

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.322	6741	1423	0.380
2	16.201	4068	818	0.229
3	16.572	3385	762	0.191
4	16.750	1691009	298890	95.374
5	17.297	4854	1107	0.274
6	17.517	1079	350	0.061
7	17.714	17670	3813	0.997
8	18.190	33702	6764	1.901
9	18.430	3203	660	0.181
10	18.832	7321	1198	0.413
Total		1773032	315785	100.000