

Sample Name : β -Endorphin, human
 Cat. No. : RP11344
 Lot. No. : E5545919H
 Time Processed :12:59:59
 Month-Day-Year Processed :09/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

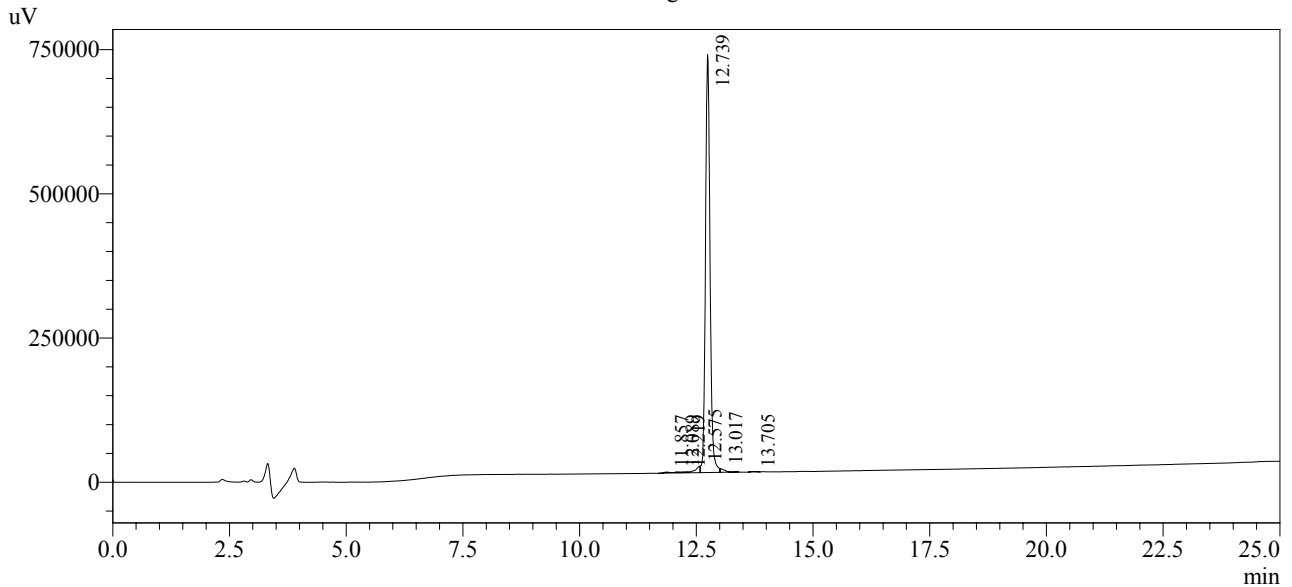

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.857	15773	1794	0.310
2	12.089	14111	1937	0.278
3	12.219	15318	1759	0.301
4	12.575	82271	11272	1.619
5	12.739	4905905	724960	96.527
6	13.017	41545	6483	0.817
7	13.705	7484	969	0.147
Total		5082408	749174	100.000