

Sample Name:Glucagon-Like Peptide (GLP) I (7-36), amide, human

Cat No:RP10773

Lot No :E3962720K

Time Processed :6:56:00 PM

Month-Day-Year Processed :11/18/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min


Wavelength:220 nm

Time	Module	Command	Value
0.10	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

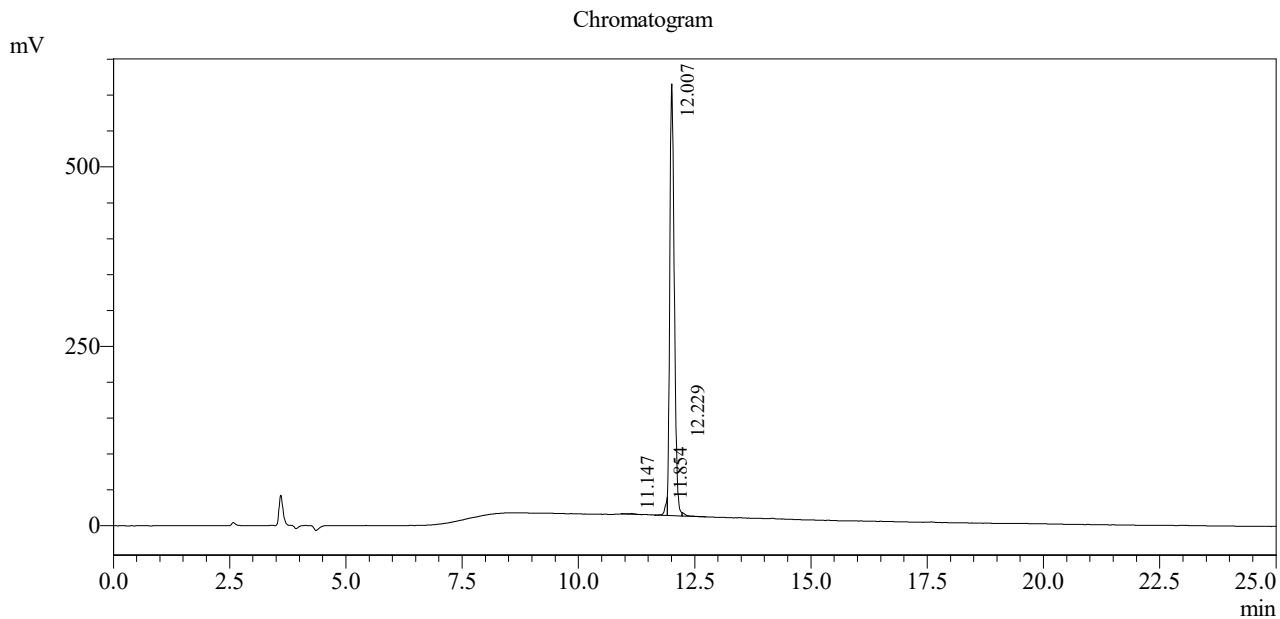

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.147	7858	928	0.188
2	11.854	73180	7774	1.751
3	12.007	4075167	601546	97.491
4	12.229	23859	4932	0.571
Total		4180064	615180	100.000