

Sample Name :HA Peptide
 Cat No.: RP11735
 Lot No.: E8589220E
 Time Processed :23:58:26
 Month-Day-Year Processed :05/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

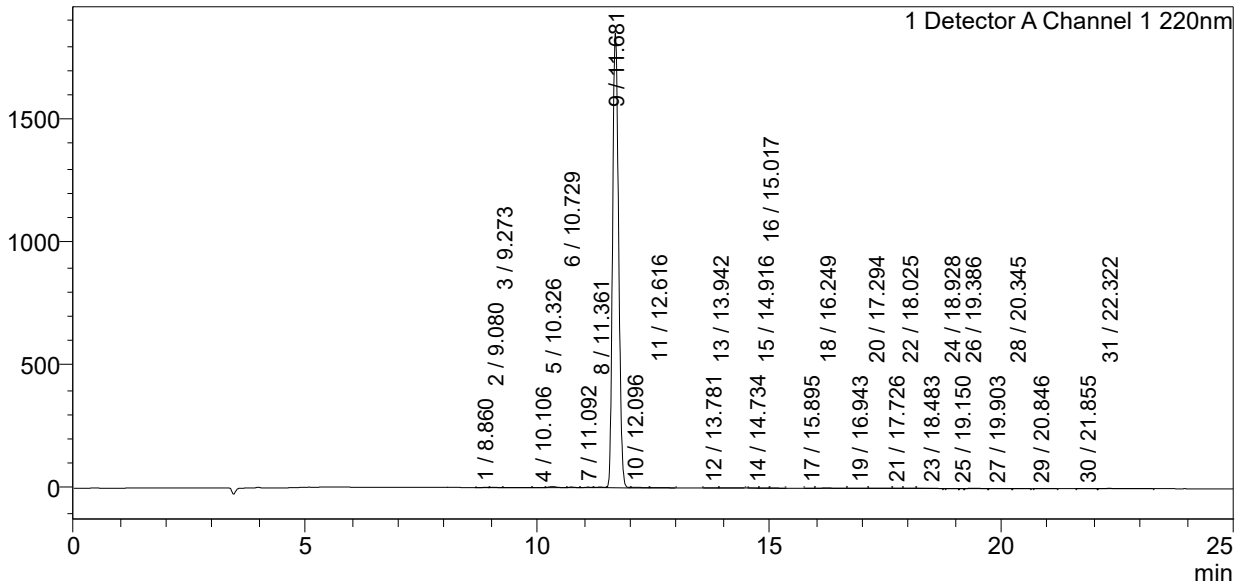

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.860	6358	533	0.037
2	9.080	10187	715	0.059
3	9.273	12724	601	0.074
4	10.106	6507	628	0.038
5	10.326	60546	4735	0.354
6	10.729	30242	3170	0.177
7	11.092	27199	2773	0.159
8	11.361	36454	2731	0.213
9	11.681	16731217	1851099	97.690
10	12.096	39580	2387	0.231
11	12.616	13742	728	0.080
12	13.781	5537	439	0.032
13	13.942	7462	367	0.044
14	14.734	3458	403	0.020
15	14.916	5551	465	0.032

Peak#	Ret. Time	Area	Height	Area%
16	15.017	4812	470	0.028
17	15.895	2409	255	0.014
18	16.249	20750	882	0.121
19	16.943	8854	532	0.052
20	17.294	13531	576	0.079
21	17.726	1403	164	0.008
22	18.025	2812	443	0.016
23	18.483	14165	801	0.083
24	18.928	2968	265	0.017
25	19.150	1203	194	0.007
26	19.386	13879	789	0.081
27	19.903	5684	324	0.033
28	20.345	1423	129	0.008
29	20.846	2231	164	0.013
30	21.855	4763	320	0.028
31	22.322	29157	1144	0.170
Total		17126807	1879224	100.000