

Sample Name :OVA Peptide (257-264)
 Cat. No. : RP10611
 Lot. No. : E7066421D

Time Processed :4:28:32 AM

Month-Day-Year Processed :04/04/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ17010508

<Chromatogram>

mV

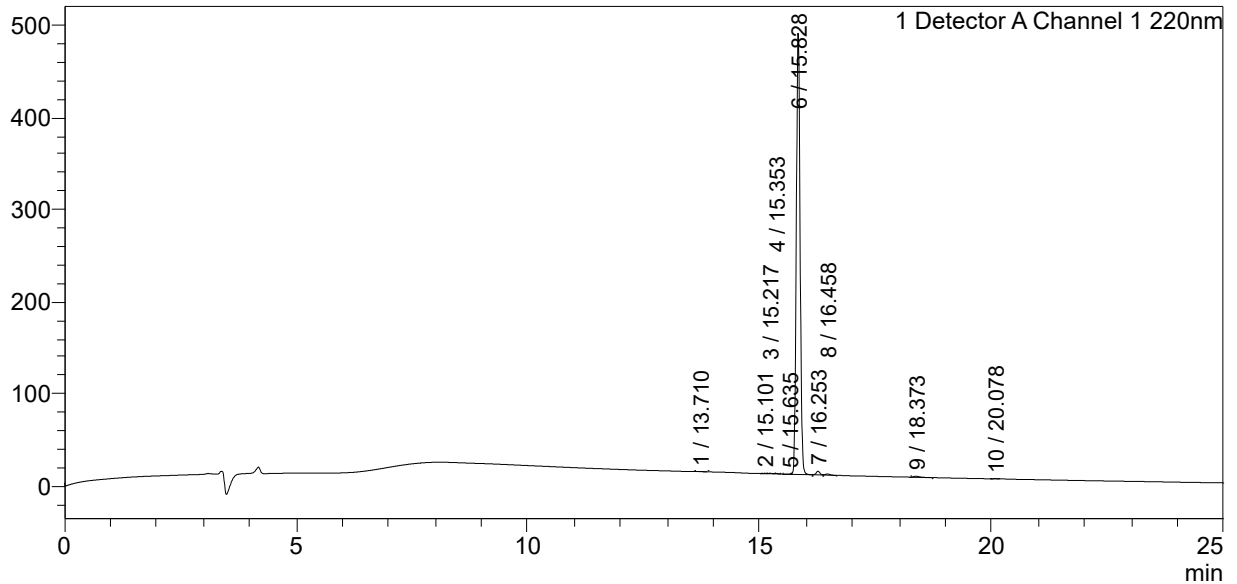

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.710	1585	234	0.057
2	15.101	2029	395	0.073
3	15.217	2101	456	0.075
4	15.353	2136	501	0.077
5	15.635	2263	406	0.081
6	15.828	2729607	478688	98.101
7	16.253	22461	3977	0.807
8	16.458	8533	1333	0.307
9	18.373	10295	1180	0.370
10	20.078	1448	262	0.052
Total		2782457	487433	100.000